

VACUUM CONTROLLER

CVC 3000



Instructions for use



Original instructions Keep for further use!

This manual is only to be used and distributed in its complete and original form. It is strictly the user's responsibility to carefully check the validity of this manual with respect to the product.

Manufacturer:

VACUUBRAND GMBH + CO KG
Alfred-Zippe-Str. 4
97877 Wertheim
GERMANY

Phone:

Head office +49 9342 808-0
Sales +49 9342 808-5550
Service +49 9342 808-5660

Fax: +49 9342 808-5555

Email: info@vacuubrand.com

Web: www.vacuubrand.com

*Thank you for purchasing this product from **VACUUBRAND GMBH + CO KG**. You have chosen a modern and technically high quality product.*

TABLE OF CONTENT


1	Introduction	7
1.1	User information	7
1.2	About this document.	8
1.2.1	Display conventions	8
1.2.2	Symbols and icons	9
1.2.3	Handling instructions (action steps).	10
1.2.4	Abbreviations	11
1.2.5	Term definition	11
2	Safety instructions	12
2.1	Working conditions	12
2.1.1	Intended use	12
2.1.2	Improper use.	12
2.1.3	Foreseeable misuse	13
2.2	Target groups	14
2.2.1	User permissions	14
2.2.2	Personal responsibility	14
2.3	Safety precautions	15
2.3.1	Protective clothing.	15
2.3.2	Eliminate sources of danger	15
2.4	Safety and service	18
2.4.1	Meaning Health and Safety Clearance	18
2.4.2	Requirements for services	19
2.5	Environmental protection	20
3	Product description	21
3.1	Vacuum controller CVC 3000	21
3.2	Functionality	23
3.3	Operation modes	24
4	Installation and connection	25
4.1	Installation	25
4.1.1	Table top version.	25
4.1.2	Built-in version	26
4.1.3	Direct installation.	26
4.1.4	Examples of use	27
4.2	Connection	29
4.2.1	Electrical connection.	29
4.2.2	Vacuum connection	31
4.2.3	VACUU·BUS®	33

5	Operating and display elements	35
5.1	Operating elements	35
5.1.1	Selection knob	35
5.1.2	Control panel	35
5.1.3	Key combinations	36
5.2	Display and user interface	37
5.2.1	Pressure display	37
5.2.2	Display icons	38
5.2.3	Signal sounds (warning beep)	40
5.2.4	Menu display in general	41
5.3	Handling CVC 3000	42
6	Operation	45
6.1	Switch-on/-off controller	45
6.2	Select language and pressure unit	46
6.3	Mode – Operation mode	47
6.3.1	Select operation mode	47
6.3.2	Mode menu	48
6.4	Start controlling	49
6.5	Control during operation	49
6.5.1	Venting (VENT)	49
6.5.2	Change operation mode	51
6.5.3	Display graphic (curve)	53
6.5.4	Quit display graphic	54
6.6	Quick adaption during operation	55
6.6.1	Set vacuum	55
6.6.2	Motor speed (only VARIO®)	56
6.7	Stop control	56
7	Advanced menus and operation	57
7.1	Operation menus	57
7.1.1	Pump down	58
7.1.2	Vac control	59
7.1.3	Auto mode (only valid for VARIO® pump)	60
7.1.4	Program	61
7.1.5	VACUULAN	62
7.2	Program functions	63
7.2.1	Open/Change program	63
7.2.2	Edit program	64
7.2.3	Store program	70
7.2.4	Display during operation	71
7.2.5	Program memory	72
7.2.6	Program examples	74
7.2.7	Sample form for program	76

7.3	Configuration menu	77
7.3.1	Content selection	78
7.3.2	Submenus	79
7.4	Function menu	82
7.4.1	Content selection	83
7.4.2	Submenu Vacuubus (address assignment)	85
7.4.3	Possible address configurations	88
7.5	Differential pressure measurement	89
8	Resolving problems	90
8.1	Error display	90
8.2	Fault – Cause – Remedy	92
8.3	Controller Reset	96
8.4	Error of external components	98
9	Cleaning and maintenance	99
9.1	Cleaning	99
9.1.1	Controller	99
9.1.2	Venting valve	99
9.1.3	Internal sensor	99
9.2	Sensor readjustment	100
10	Appendix	103
10.1	Technical information	103
10.1.1	Technical data	103
10.1.2	Product comparison CVC 3000	105
10.1.3	Rating plate	106
10.1.4	Wetted parts	106
10.2	Interface commands	107
10.2.1	Pin assignment (RS232)	107
10.2.2	Read commands (CVC 2000)	108
10.2.3	Write commands (CVC 2000)	109
10.2.4	Read commands (CVC 3000)	110
10.2.5	Write commands (CVC 3000)	113
10.3	Ordering information	115
10.4	Service	117
10.5	Glossary	118
10.6	Index	119
10.7	Certifications	121
10.7.1	EC Declaration of Conformity	121
10.7.2	UKCA Declaration of Conformity	122
10.7.3	US/CAN Certificate	123
10.7.4	Declaration of Conformity – China RoHS 2	124

First steps (delivery status)

First steps on
delivery status
Select language and
units

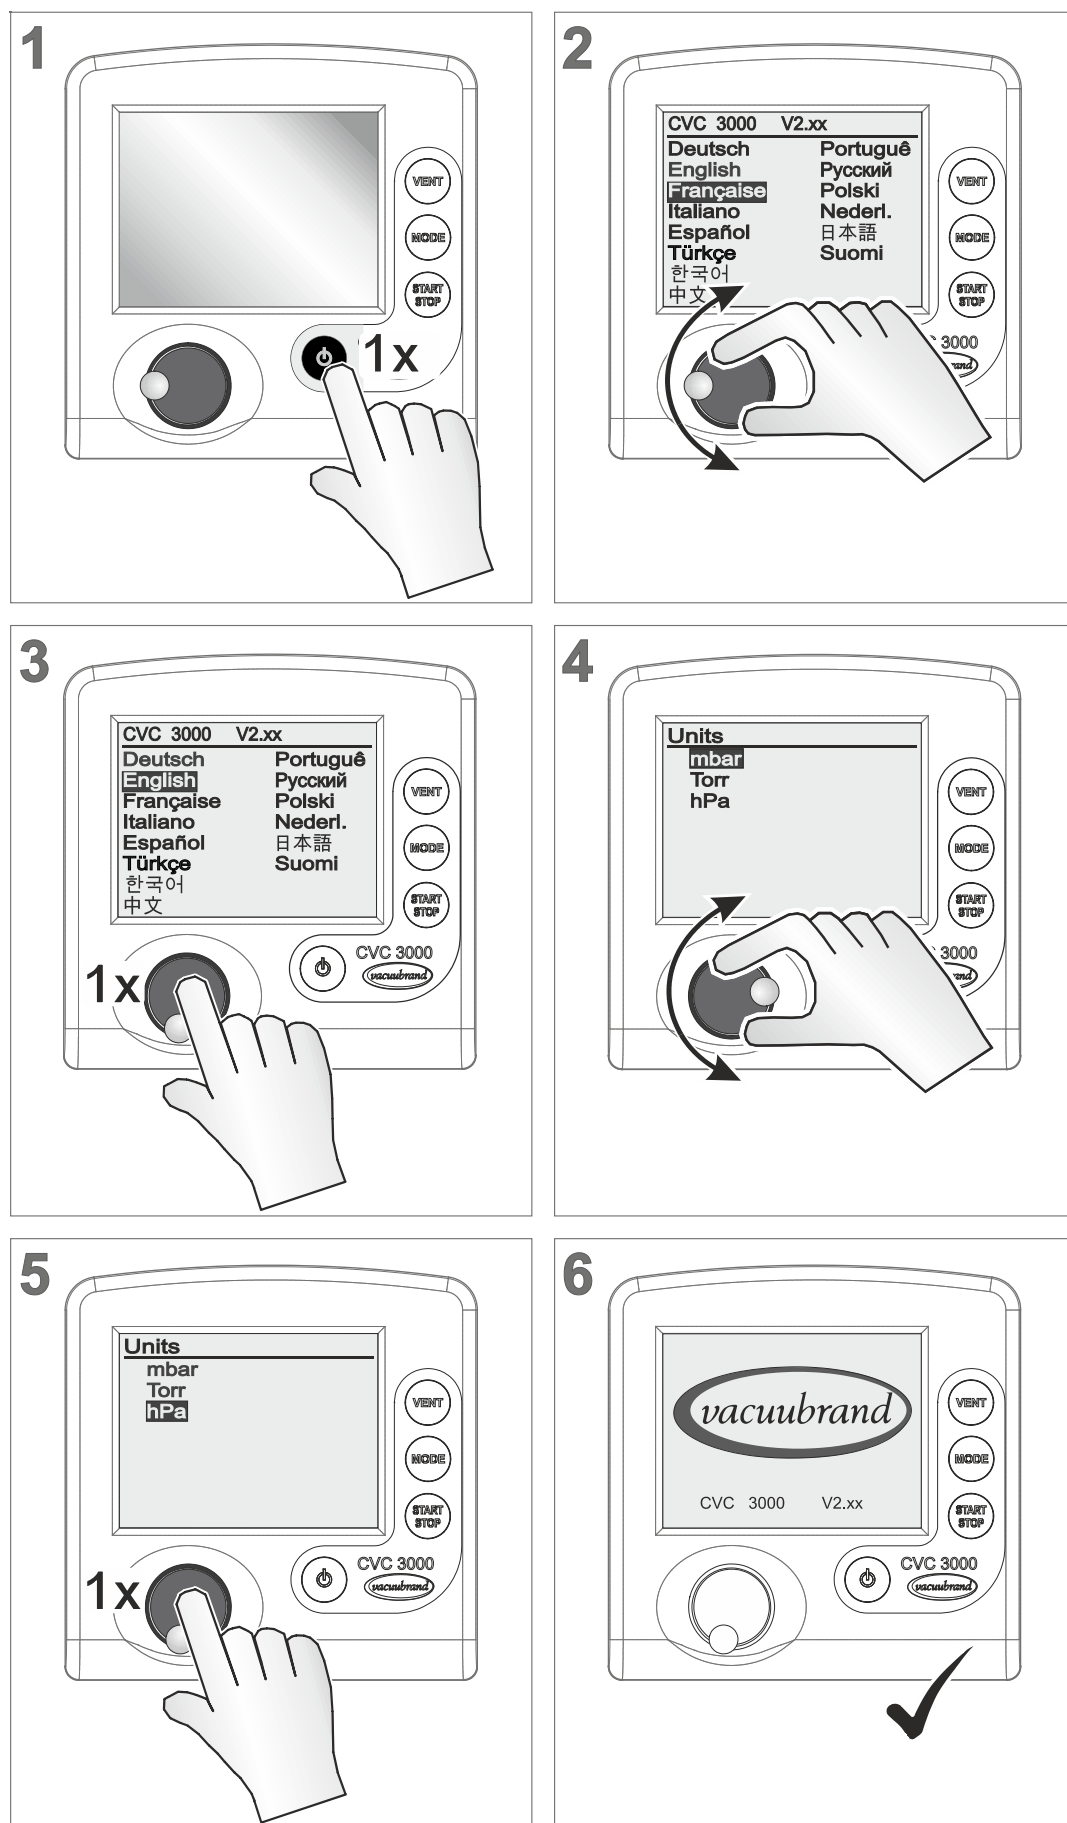

1 Introduction

This manual is part of your product. It provides important instructions for safe use of the product. Read this manual completely in order to understand proper use of your product.

1.1 User information

Safety

Instructions for use
and safety

- Read this manual thoroughly and completely before using the product.
- Keep this manual in an easily accessible location.
- Proper use of the product is essential for safe operation. Comply with all safety instructions provided!
- In addition to this manual, adhere to any relevant local accident prevention regulations and comply with industrial safety regulations.

General

General
information

- To make the text more readable in this manual, mostly the term **Controller** is used instead of **CVC 3000**.
- When giving the product to a third party also hand out these instructions for use.
- The illustrations in this manual are provided as examples. They are intended to aid in your understanding of the proper use of the product.
- **VACUUBRAND GMBH + CO KG** reserves the right to modify or change the product design and/or technical specifications at any time without advanced notice.

Copyright

Copyright ©

The content of these instructions for use is protected by copyright. Only copies for internal use are allowed, e. g., for professional training.

© **VACUUBRAND GMBH + CO KG**

Contact

Contact us




- Please ask for replacement in case of an incomplete manual or download instructions for use on our web page: www.vacuubrand.com
- Contact us regarding any questions about this product, if you need further information, or to provide us with feedback.
- When contacting our Customer Service Department, please be sure to have the correct type and serial number of your product → see *Rating plate*.

1.2 About this document

1.2.1 Display conventions

Warning levels

Convention for warnings

	DANGER Indicates an imminent hazardous situation. Disregarding the situation will result in serious and even fatal injury or death. ⇒ Take appropriate action to avoid dangerous situation!
	WARNING Indicates a potentially hazardous situation. Disregarding the situation could result in serious, even fatal injury or massive damage to property. ⇒ Observe instruction to avoid dangerous situation!
	CAUTION Indicates a potentially hazardous situation. Disregarding the situation could result in slight or minor injury or damage to property. ⇒ Observe instruction to avoid dangerous situation!

Convention for
additional notes

NOTICE

Notice for a potentially harmful situation.

Disregarding the notice could lead to material damage.

Additional notes

IMPORTANT!

⇒ Information or specific use recommendation, which must be observed.

⇒ Important information for the proper operation.



⇒ Helpful tips and tricks

⇒ Additional information

1.2.2 Symbols and icons

This manual includes symbols and icons. Safety symbols indicate special danger in handling the product. They shall help to identify the danger directly and easier.

Safety symbols

Explanation of safety
symbols



acute toxicity – hazards
to human health



general warning symbol



danger: electricity



hot surface



general prohibition
symbol














general mandatory sign



disconnect mains plug
from outlet

Additional icons

References		Positive example – Do! result – o. k.		Negative example – Do not!
		Refers to content of this manual.		Refers to content of other documents.
Handling or action		Press selection knob or key.		Turn selection knob
		Push and hold key		Push and turn selection knob
Signals		Flashing cycle – flashing icon indicating malfunction		
		Sound – signal or warning sound		
		Electric/electronic devices and batteries must not be disposed of in the domestic waste at the end of their service life.		



⇒ For further detailed information about icons and signals in the display see chapter **5.2.2 Display icons**.

1.2.3 Handling instructions (action steps)

Design of action
steps

Action step (single step)

⇒ Do the described step.

☒ Result of action.

Action step (multiple steps)

1. First step,


2. next step.

☒ Result of action.

Follow steps in the described order.

1.2.4 Abbreviations

Abbreviations

abs.	Absolute
ATM	Standard Atmospheric Pressure
CVC 3000	Controller
d_i (di)	Interior diameter
DN	Nominal diameter
	ATEX equipment labeling
EK	Emission condenser
EX*	Outlet
FKM	Fluoroelastomer
Gr.	Size
hh:mm:ss	Time settings in hour/minute/second
hPa	Pressure unit, hectopascal (1 hPa = 1 mbar = 0.75 Torr)
IN*	Inlet
KF	Small flange
max.	Maximum value
mbar	Pressure unit, millibar (1 mbar = 1 hPa = 0.75 Torr)
min.	Minimum value
Min	Minute
PA	Polyamide
PBT	Polybutylene terephthalate
PE	Polyethylene
respon.	responsible, supervising Specialist
RMA-N°	Return Merchandise Authorization number
SW	Wrench size (tool)
Torr	Pressure unit (1 Torr = 1.33 mbar = 1.33 hPa)
VAC	Vacuum
VMS	Vacuum Management System

* labeling on top of the vacuum pump

1.2.5 Term definition

Product specific terms

...-I/O module	Interface for an external peripheral device to connect with a VACUU·BUS® capable vacuum gauge or -controller
VACUU·BUS®	Bus system by VACUUBRAND.
VACUU·CONTROL®	Web-based application as remote control for vacuum controller and gauges made by VACUUBRAND.
VACUU·LAN®	Local vacuum network for laboratories.
VARIO® control	Precise vacuum control by motor speed control of VARIO® diaphragm pumps.

2 Safety instructions

All safety instructions must be observed by all individuals working with the product described here. The safety instructions are valid for the complete life cycle of the product.

2.1 Working conditions

Use the product only when it is in proper working condition.

2.1.1 Intended use

Intended use The **Controller CVC 3000** is a laboratory instrument, used to measure and/or control vacuum in therefore intended plants. The controller may only be used in non-explosive areas and indoors. Any other use is considered to be improper use. In that case, the safety and the protection of the system may be compromised.

Intended use also includes the following:



- observing safety information of document “**Safety Information for Vacuum Equipment**“.
- observing this manual.
- observing the manual of connected elements and to know their functioning.

2.1.2 Improper use

Using the product in contrary to its intended use could result in injury or damage to property.

Improper use includes:

- Improper use
- Using the product contrary to its intended use.
 - Operation with obvious malfunctions.

Improper use

- Controlling explosive atmosphere, which does not compare to the ATEX approval of the **CVC 3000** → *see rating plate*.
- Unauthorized modifications and the use of accessories and spare parts that are not recommended by the manufacturer.
- Use in mining.

2.1.3 Foreseeable misuse



Additionally to improper use there are types of use and dealing with the product, which are generally prohibited:

Reasonably
foreseeable
misuse

- The control of media which is liquid, hot, instable, or explosive.
- Installation and operation in explosive environments.
- To switch on/-off by foot or with unsuitable tool.
- To operate the controller with sharp stylus or objects.
- To put the controller completely into vacuum.
- To immerse the controller into liquid or to blast it with steam.
- To use the remote control **VACUU·CONTROL[®]** with CVC 3000 without knowledge of the connected vacuum system.

2.2 Target groups

IMPORTANT!

Ensure that the controller is only operated by authorized and skilled personnel.

Users need to have the corresponding skills and qualifications for doing the job listed in the table *User permissions*.

2.2.1 User permissions

This manual must be read, understood and complied with by the person performing one of the following tasks:

Responsibility
Assignment Matrix

Task (Job)	User	Specialist	Supervising Specialist
Installation and assembly		X	X
Commissioning		X	X
Operation	X	X	X
Readjust vacuum sensor		X	X
Error report	X	X	X
Troubleshooting		X	X
Update		X	X
Cleaning, simple	X	X	X
Clean vacuum sensor		X	X
Decontamination			X*
Repair order			X

* or order the decontamination by a qualified service provider.

2.2.2 Personal responsibility

Safe work

Personal safety has top priority. Processes which create a potentially hazardous situation are not allowed.

Always be conscious of safety, and work in a safe manner. Observe the owners' directives at work, the national accident prevention regulations and occupational safety provisions.

⇒ Use the controller only if you have understood its function and this manual.


2.3 Safety precautions

Quality standards
and safety

Products of **VACUUBRAND GMBH + CO KG** are subject to high quality tests with goals for safety and operation. Prior to delivery each product has been tested thoroughly.

2.3.1 Protective clothing

Protective clothing

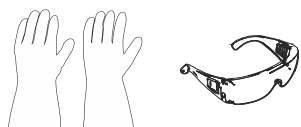

No special protective clothing is required when working with the controller. Observe the owners regulation for workplaces.

Only for cleaning the controller we recommend to wear protective gloves, protective clothing and safety goggles.

IMPORTANT!

- ⇒ Be sure to observe the local requirements for decontamination.
- ⇒ Wear your personal protective equipment when handling chemical materials.

2.3.2 Eliminate sources of danger



DANGER

Explosion hazard for critical processes.

Depending on the process explosive mixtures can develop.

- ⇒ Never operate critical processes unattended!

Explosion danger for
critical processes

Depending on the running process, explosive mixtures can form in plants or other hazardous situations could result!

IMPORTANT!

Malfunctions which may affect safety must be eliminated immediately.

- ⇒ Do not work with damaged components.
- ⇒ Replace defective parts immediately, e. g., broken cable or faulty plug-connection.

Sources of error during connection

NOTICE

Measuring error due to an obstructed vacuum line.

⇒ Prevent overpressure > 1060 mbar (> 795 Torr) in the piping system.

Condensate Condensate can falsify the measurement. Position the vacuum hose in such a way that condensate cannot flow towards the controller and its vacuum sensor. No liquid should accumulate inside the vacuum hose.

⇒ Install vacuum hoses in such a way that condensate cannot flow into the controller.

Particles, liquids, dust Particles, liquids or dust may not enter the controller.

⇒ Install a separator or filter at the intake of the system.
Appropriate filters are for example chemically resistant, and resistant to clogging.

Risks due to residual energy

Residual energy After switching off the controller and disconnecting it from mains, risk of residual energy could still prevail at the power supply adapter.

⇒ Repairs may only be performed by qualified personnel, e. g., service technician.

Option **CVC 3000 in combination with VACUU·CONTROL[®]**

VACUU·CONTROL[®] is a remote control for the controller. It is available as an accessory.

With this accessory a vacuum system can be operated simultaneously by controller or via **VACUU·CONTROL[®]**. Remote control is able to operate from several end devices, e. g., smart phone, tablet, or computer.

When using remote control please regard the following:

- ⇒ Coordinate planned projects with colleagues sharing the equipment.
- ⇒ If necessary inform colleagues that you plan to use the remote control.
- ⇒ Avoid different, parallel settings.


Installation and explosive environment

Installation and operation in areas where explosive atmospheres can occur is not allowed.

ATEX marking

ATEX category



Controllers which are labeled with  have an ATEX approval 3 G; i. e. flammable substances as mixture with air: pumped gas or vapor.

- ⇒ Use the controller only when it is in proper working condition.

ATEX approval¹ is only valid for the internal, wetted parts area (vacuum sensor), not for the environment of the controller.

ATEX category and peripherals

The ATEX category of the controller is dependent on the connected peripheral devices. Peripherals and connected devices to the controller need to have the same or must have a higher ATEX approval. Without concordant categorization of peripherals, the specified category of the VACUUBRAND equipment loses its validity.

Avoid ignition sources

The use of gas ballast or the operation of venting valves is only permitted if thereby explosive atmospheres normally do not occur in the interior of the equipment or, if they do occur, are likely to do so only infrequently and for a short period.


- ⇒ If necessary vent with inert gas.

For more and detailed information about ATEX approval visit our website: www.vacuubrand.com/Information-ATEX

¹ -> compare to rating plate

Explanation of usage
conditions X

Example extract
type plate



Restrictions on operating conditions

Meaning for devices marked with X:

- The devices have a low mechanical protection and must be installed so that they cannot be mechanically damaged from the outside; e.g., installing pump stations with impact protection, attaching shatter protection for glass flasks, etc.
- The devices are designed for an ambient and media temperature of +10 °C to +40 °C during operation. These ambient and media temperatures must never be exceeded. When conveying/measuring non-explosive gases, extended gas suction temperatures apply, see chapter: Technical information, media temperature (gas).

2.4 Safety and service

Obligations for
service jobs

Safety regulations that apply to your work environment also apply to persons who perform service works, especially in the handling of hazardous materials.

2.4.1 Meaning Health and Safety Clearance

Products which are potentially hazardous may only be returned when all dangerous contaminations are removed.

IMPORTANT!

- ⇒ Observe the requirements for services.
- ⇒ Observe the **Notes on return to the factory** listed on the form Health and Safety Clearance.
- ⇒ Protect the service personnel from hazardous substances.
- ⇒ Confirm harmlessness with your signature.



⇒ The form [Health and Safety Clearance](#) is also available on our website.

2.4.2 Requirements for services

Fulfill the following conditions

1. Clean your product thoroughly and if necessary decontaminate it professionally.

IMPORTANT!

For all service works hazardous substances need to be excluded.

2. Fill in the form *Health and Safety Clearance* thoroughly and completely.
3. Contact your local supplier or our service department.
4. Request a **RMA-N°** for your **service order**.
5. **Before returning the product**, please **send the signed *Health and Safety Clearance* form** to your local supplier or our service department.

IMPORTANT!

For all service works the safety clearance needs to be proofed and confirmed.

⇒ Did your product get in touch with hazardous substances?
Please wait for the release of reshipment.

6. Send in your product including:
 - RMA-N°,
 - Service order (e. g., repair),
 - Form *Health and Safety Clearance*,
 - Short description (e.g., malfunction, working environment, media).



Any more questions? We will help you:

Phone: +49 9342 808-5660

Fax: +49 9342 808-5555

service@vacuubrand.com

2.5 Environmental protection

NOTICE

Risk of environmental damage due to incorrect disposal of the controller.

- ⇒ Do not dispose your product in household waste!
Electronic components are subject to hazardous waste treatment and must only be disposed of by certified specialists.
- ⇒ Observe the national regulations for safe disposal and environmental protection.
- ⇒ Receive detailed information about respective regulations from your competent administrative authority.



3 Product description

Goods arrival

Check incoming
goods

Check the shipment for transport damage and completeness.
⇒ Report any transit damage immediately to the supplier.

NOTICE

Condensate can damage the controller.

A large temperature difference between storage location and installation location can cause condensation.

⇒ Let the product acclimatize for 3–4 hours.

Included materials

Scope of supply

Controller

Vacuum controller
CVC 3000

see *Ordering information on page 115*

Power supply unit 30W 24V; including interchangeable mains plugs	20612090
Instructions for use	20901067
Safety Information for Vacuum Equipment	20999254
Origin packaging	-----

3.1 Vacuum controller CVC 3000

The controller is designed for applications requiring controlled vacuum.


The controller has a two-point control mode to switch an in-line isolation valve.

The controller is freely programmable. Up to 10 programs can be stored in the controller memory. Each program also offers up to 10 program steps (time/pressure) plus control functions, such as: venting, pump down and ramp function.

The controller enables the measurement of relative pressure with regard to a reference sensor (VSK 3000).

Front

Front panel


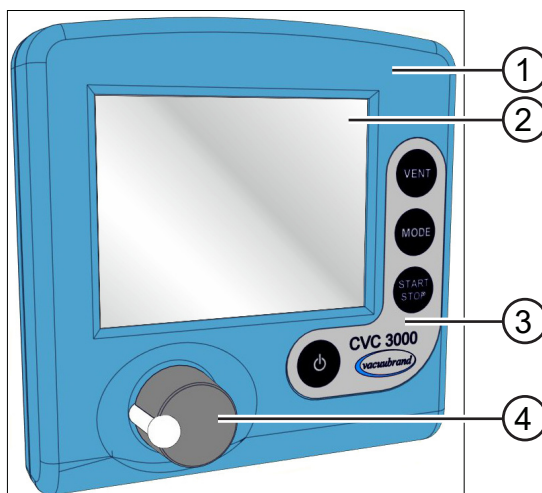


Meaning

- | | |
|---|--------------------------------------|
| 1 | Chemically resistant plastic housing |
| 2 | LC display |
| 3 | Control panel and product name |
| 4 | Selection knob |

Rear side

Rear side

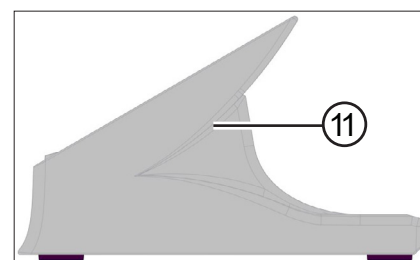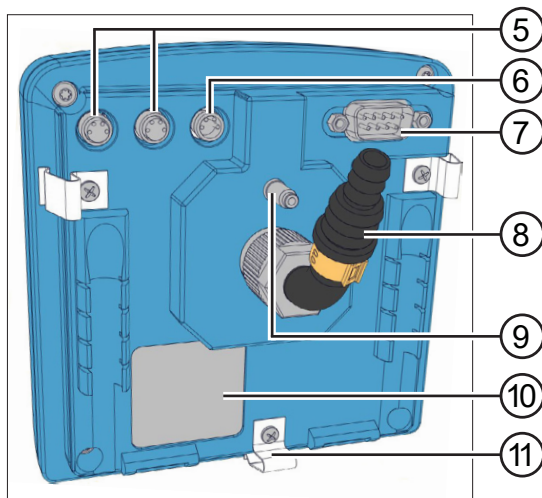

Meaning

- | | |
|----|--|
| 5 | Ports for VACUUBUS® components |
| 6 | Mains connection
▶ power supply unit
▶ VARIO® diaphragm pump or
▶ pumping system |
| 7 | Serial port RS 232 C (Sub-D) |
| 8 | Hose nozzle, vacuum connection |
| 9 | Venting tube, connection for external venting, e. g., inert gas |
| 10 | Rating plate |
| 11 | Spring clip as fixation for built-in version
or
plastic foot for table top version |

3.2 Functionality

Functionality

The controller manages vacuum processes by controlling vacuum pumps, in-line isolation- and/or air admittance valves. It controls process vacuum, cooling water and venting to demand.



Valves and/or vacuum pumps are necessary to operate the controller.

Without those components the controller can only be used as vacuum measurement device.

Specification

Specification and features

- Ceramic diaphragm vacuum sensor¹ and venting valve are already integrated into the controller.
- The ceramic vacuum sensor is chemically highly resistant, measures accurately and is gas-type independent.
- External valves, level sensors and vacuum sensors can be connected directly by **VACUU-BUS[®]** system, e. g., vacuum-, in-line isolation-, cooling- and air admittance valves as well as level sensors and emission condenser **Peltronic[®]**.
- While booting the controller checks for current configuration of connected components.
- Connected components are detected automatically due to **VACUU-BUS[®]** and controlled by the controller until the controller is switched off. Safety sensitive components stay configured and are monitored again after controller restart.
- Operating elements are the selection knob, buttons on the control panel and full text menus on the display.
- Port RS 232 can also be used for connecting the remote control **VACUU-CONTROL[®]**. The controller can be operated by one or several end devices, e.g., smartphone, tablet, computer.



¹ -> excluded for package fine vacuum control with VSP 3000.

3.3 Operation modes

Up to 5 different operation modes are selectable at the controller. Specific modifications can be realized by individual mode menus.

Selectable operation modes

- Standard
- **Pump down**
 - **Vac control**
 - **Program**

- Optionally
- **Auto mode**
 - **VACUULAN**

For more information about individual operation modes
→ see chapter **6.3.2 Mode menu**

4 Installation and connection

The controller is designed for installation directly at the workplace.



⇒ Observe all specifications for installation, connection and operation according to technical data,
→ see *chapter 10.1.1 Technical data*.

⇒ Also observe rating plate data.

Installation conditions

Consider installation conditions

- The controller has acclimatized.
- Ambient conditions are observed and are within the limitation of use.

Limitation of use		(US)
Ambient temperature	10–40 °C	50–104°F
Altitude, max.	3000 m above sea level	9840 ft above sea level
Relative humidity	30–85 %, non condensing	
Degree of protection (controller front)	IP 20 (IP 42)	
Avoid condensation or contamination by dust, liquids or corrosive gases.		

4.1 Installation

4.1.1 Table top version




The table top or bench-top type controller can be installed and connected directly on top of the work bench or on laboratory table. The table top version is supplied with a hose nozzle. The hose nozzle should be positioned in a way that the connected vacuum hose cannot kink.

4.1.2 Built-in version



The CVC 3000 can be used as built-in version fixed with spring clips; e. g., as front controller of a **VARIO**® pump, built into a cable duct cover or into the cut-out of a switch cabinet.

Cut-out for switch cabinet or cable duct cover

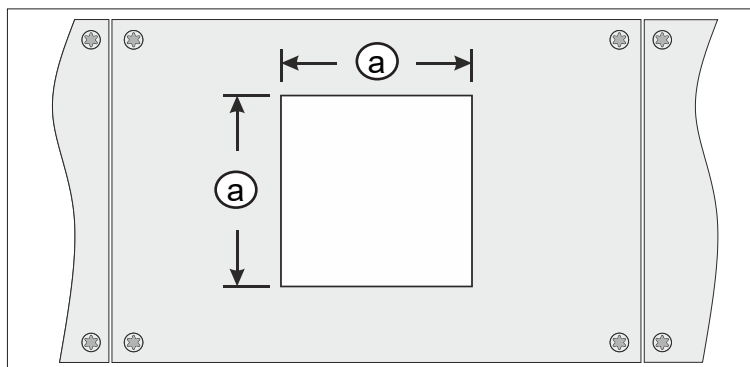

Thickness		Size (a) for cut-out	
1 mm	0.04 in.	111,5 mm x 111,5 mm	4.39 in. x 4.39 in.
2 mm	0.08 in.	112 mm x 112 mm	4.41 in. x 4.41 in.
3 mm	0.12 in.	112,5 mm x 112,5 mm	4.43 in. x 4.43 in.

Depending on the wall thickness the cut-out size needs to be fitted.


4.1.3 Direct installation

The controller can be mounted directly at the vacuum vessel using a clamping ring

→ see also example *CVC 3000 directly mounted on page 28.*


4.1.4 Examples of use

→ Example
VARIO® pump with
CVC 3000 and
rotary evaporator

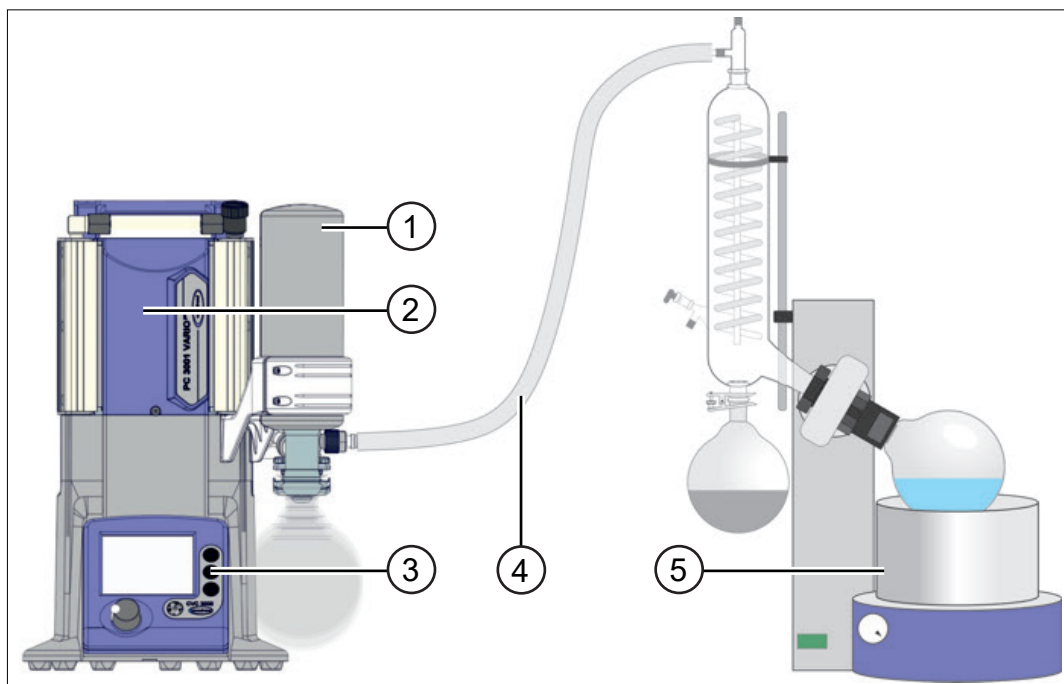


- 1 Emission condenser with round flask
- 2 **VARIO®** pump (PC 3001 **VARIO®**pro)
- 3 Controller CVC 3000, built-in version
- 4 Vacuum hose
- 5 Rotary evaporator

→ Example
CVC 3000 build-up
with cabinet dryer

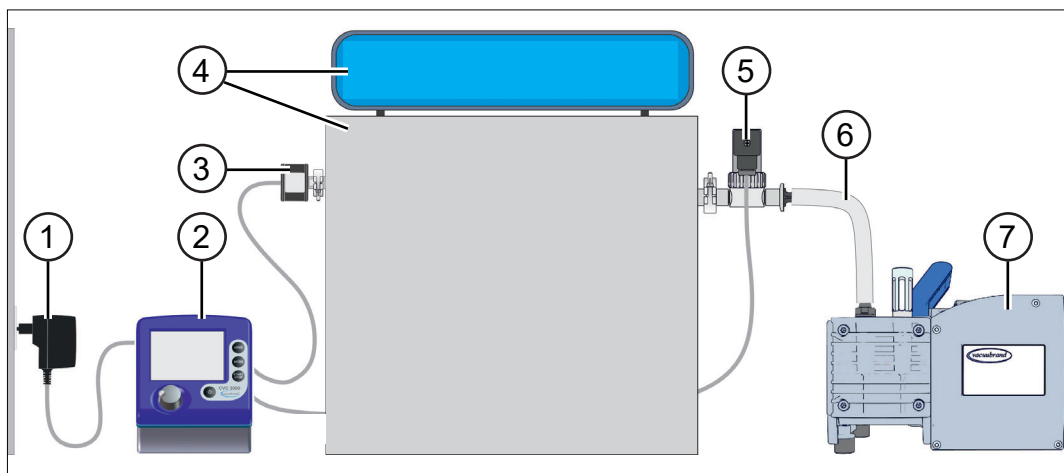

- 1 Wall power supply
- 2 Controller CVC 3000, table top version
- 3 Vacuum sensor (VSK)
- 4 Cabinet dryer with control unit on top
- 5 Vacuum valve
- 6 Vacuum hose
- 7 Diaphragm pump, vacuum pump

→ Example
CVC 3000 directly
mounted

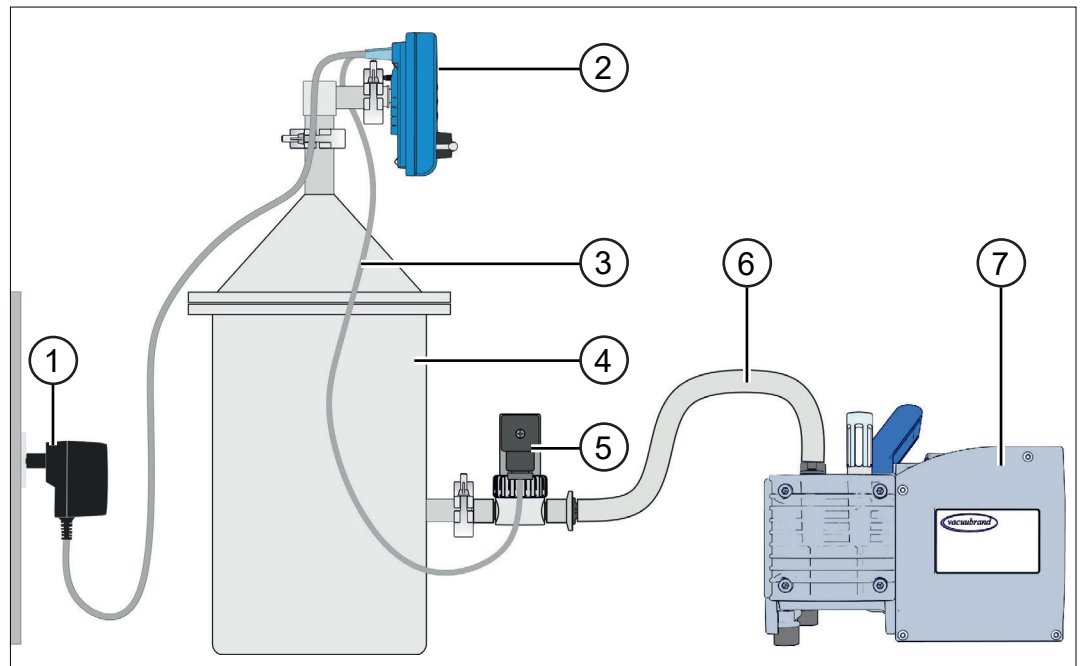

- | | |
|---|---------------------------------------|
| 1 | Wall power supply |
| 2 | Controller CVC 3000, directly mounted |
| 3 | VACUU-BUS® cable |
| 4 | Vacuum vessel, recipient |
| 5 | Vacuum valve |
| 6 | Vacuum hose |
| 7 | Diaphragm pump, vacuum pump |



⇒ Install the controller as close as possible to the process in order to optimize vacuum control.

4.2 Connection

4.2.1 Electrical connection


NOTICE

The CE/UKCA mark and a cTÜVus mark (see rating plate) may be voided if not using a VACUUBRAND power supply.

- ⇒ Use a VACUUBRAND wall power supply plug or another VACUUBRAND peripheral device (e. g., Chemistry pumping unit PC 3001 VARIO^{pro}) to provide the supply voltage.
- ⇒ If the supply voltage is not provided by VACUUBRAND wall power supply plug or any other VACUUBRAND peripheral device (e. g., Chemistry pumping unit PC 3001 VARIO^{pro}), the power supply must provide a stabilized 24 V DC voltage which must not provide more than 6.25 A even in case of failure.
- ⇒ If using additional overcurrent protection devices (e. g., fuses), these protection devices must interrupt the supply voltage at a maximum current of 8.4 A after 120 s at the latest.

Wall power supply kit*

Power supply kit
for CVC 3000

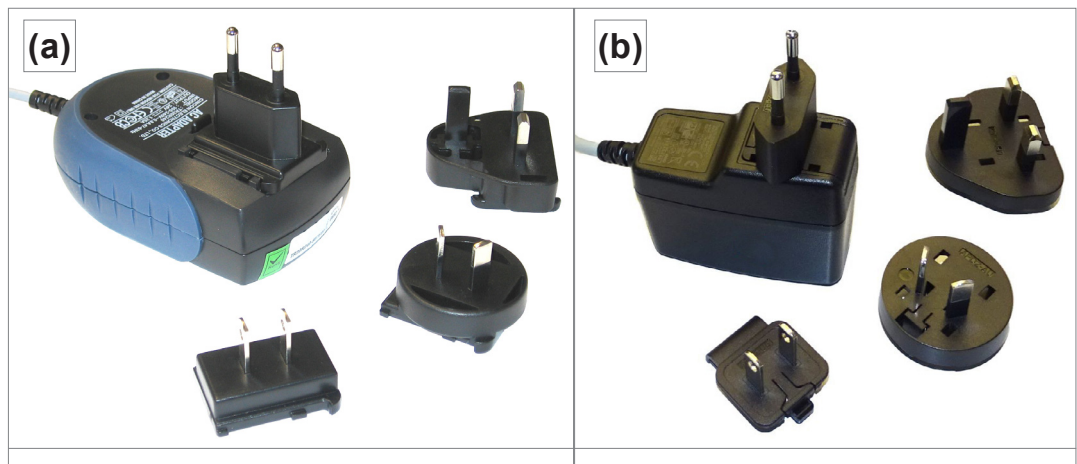

* Short-circuit-proofed multi-voltage power supply with integrated overload protection and changeable mains plugs:

(a) valid until 11/2020

(b) valid from 12/2020

Prepare wall power supply plug

Prepare connection

1. Take the wall power supply kit out of the packaging.
2. Select the mains plug that fits to your mains socket.

3. Connect the mains plug to the metal contacts of the wall power supply plug.
4. Slide the mains plug until it locks.

Remove mains plug

Remove mains plug


1. Press the locking knob on top of the wall power supply plug.
2. Remove the mains plug.

☑ Another mains plug can be fixed.

Connect power supply to the controller

⇒ Plug female connection of the power supply cable into mains connection of the controller.

Mains connection on the rear side

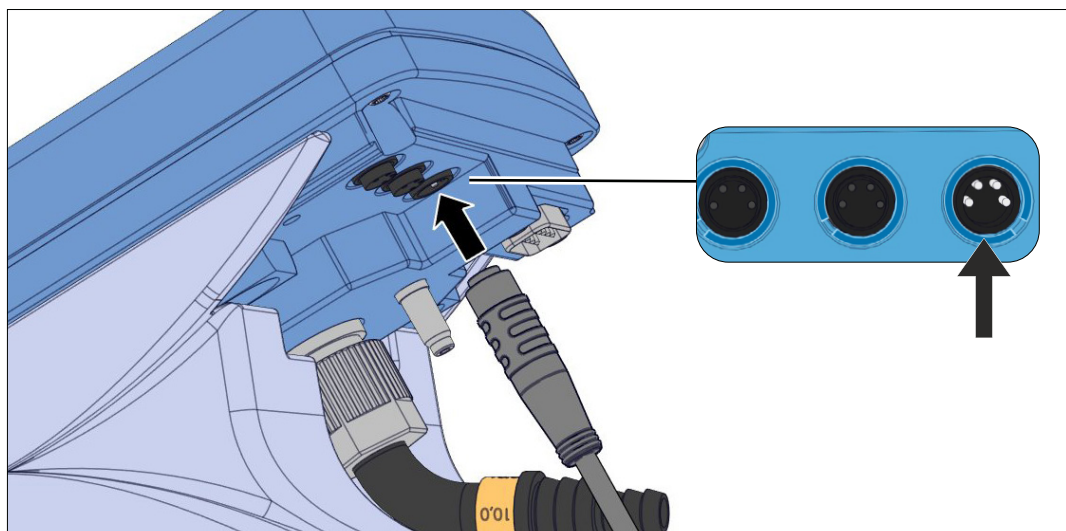


Ports with guide groove

Consider new connection design:


For easy connection, the CVC 3000 of the newest series have a guide groove on the rear side for each port.

For connection insert the nose of the round plug into the guide groove.

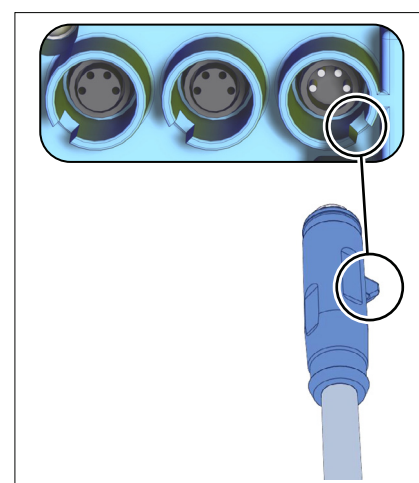

IMPORTANT!

- ⇒ Please install the power supply line in such a way, that no damage be caused to the cable due to sharp edges, chemicals or hot surfaces.

**Connect to mains**

- ⇒ Plug the wall power supply into the mains socket.

4.2.2 Vacuum connection**NOTICE****Flexible vacuum hoses can contract because of evacuation.**

- ⇒ Fix vacuum hose at the connections.
- ⇒ Fix connected components.
- ⇒ Measure and trim the vacuum hose to a length that cares for the maximum shrinkage.

Possible damages to parts which are in contact with process media.

Residuals of aggressive or condensing media can cause damages to the controller or its inner parts.

- ⇒ Prevent that damaging process media can get into the controller.

Filters will compromise measurement and control.

Connect vacuum line

- ⇒ Connect the vacuum line gas-tight to the vacuum port of the controller;
→ see also *Connection examples on page 32*.



IMPORTANT!

- ⇒ Only use a vacuum hose that is sufficient for the purpose and which provides enough stability.
- ⇒ Use hose tubes as short as possible.
- ⇒ Maximum admissible pressure at vacuum sensor:
1,5 bar/ 750 Torr (absolute).
- ⇒ Observe the maximum measuring limit of the controller, approximately 1060 mbar (795 Torr).

Connection examples



Depending on design and installation the controller provides several options for connection to the vacuum system.

Table top version

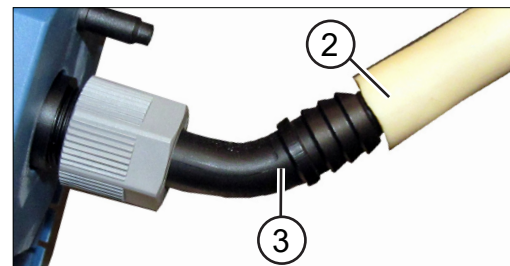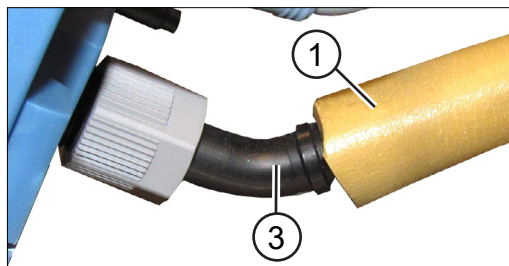



- Flexible caoutchouc hose (1) or (2), directly plugged on the **hose nozzle (3)**.

Direct installation

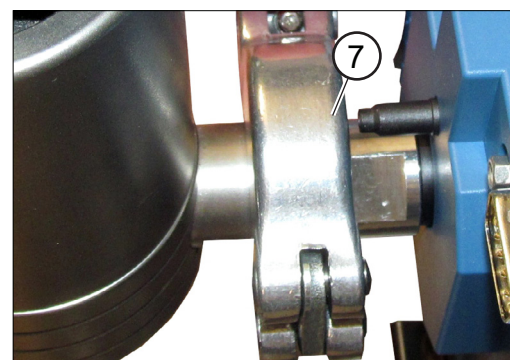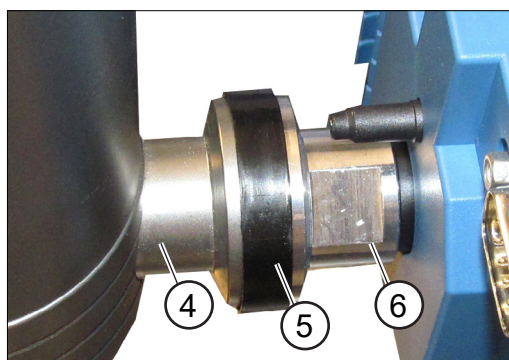

- Flange connection (4)** at vacuum chamber with sealing ring (5) and small flange (6) screwed to CVC 3000 fixed with clamping ring (7).

Built-in version
(front mounting)

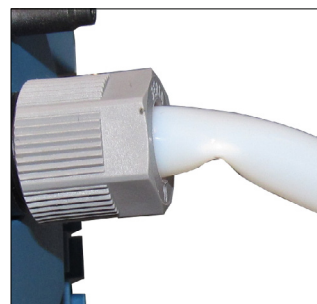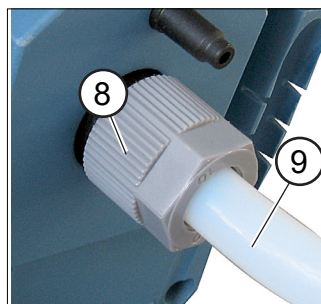

- Vacuum hose made of PTFE (9) – plugged on **hose nipple**, fixed with union nut (8).


IMPORTANT!

With built-in controller the vacuum port is not visible. The vacuum hose may not be kinked.

- ⇒ Make sure there is sufficient space inside the housing, or
- ⇒ use a stable, curved hose nozzle for connection.

4.2.3 VACUU·BUS®

Meaning and
functioning




VACUU·BUS® is a system for communication to peripheral accessories which can be directly connected to the controller. These accessory components are self-configuring by switching on the controller. All **VACUU·BUS®** components are compatible to the controller.

Two ports on the rear of the controller are for connection of **VACUU·BUS®** components. These plug-and-socket connections and Y adapters make it possible to connect up to 32 accessory components.

VACUU·BUS® principle

→ Example
Principal sketch

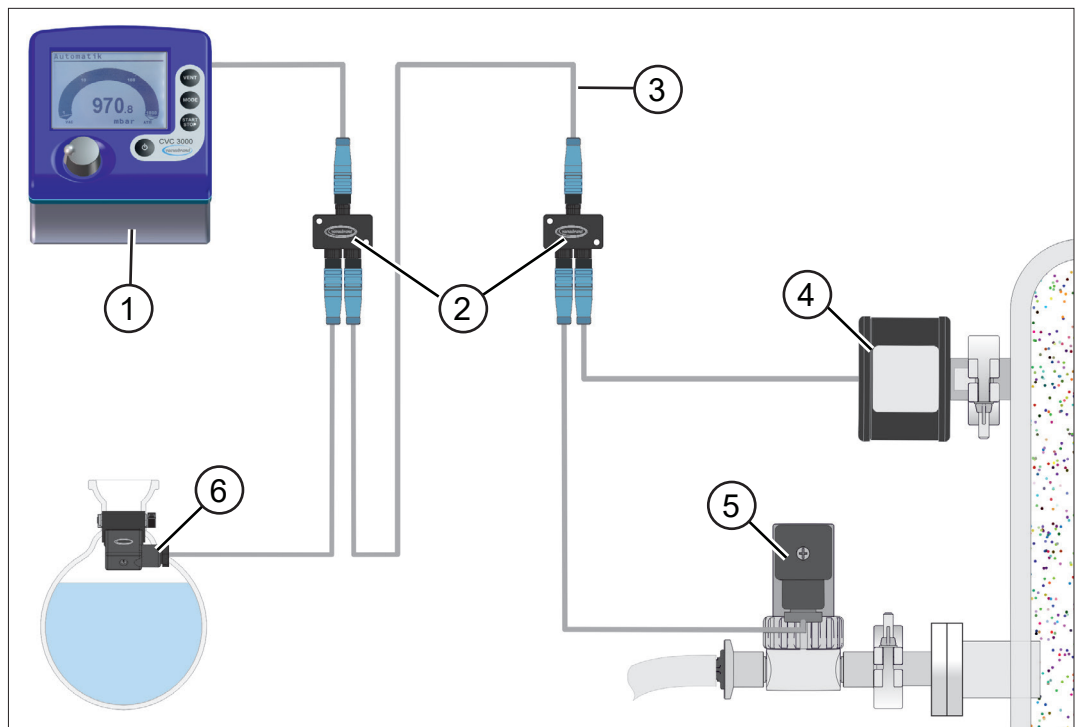

VACUU·BUS®
components

1 CVC 3000	4 Vacuum sensor VSK
2 Y adapter	5 Vacuum valve (In-line valve)
3 Extension cable	6 Level sensor

IMPORTANT!

⇒ When connecting multiple, identical **VACUU·BUS®** components, e. g., 3 external vacuum sensors VSK, those first need to be assigned different addresses, in order to avoid communication faults. → see *chapter 7.4.2 Submenu Vacuubus (address assignment)*.

VACUU·BUS® components

VACUU·BUS®
accessories
(Option)

Vacuum sensor	VSK 3000	20640530
	VSP 3000	20636163
	VACUU·SELECT Sensor	20700020
	VACUU·SELECT Sensor without venting valve	20700021
Vacuum gauge	VACUU·VIEW	20683220
	VACUU·VIEW extended	20683210
Vacuum valve (In-line valve)	VV-B 6	20674290
	VV-B 6C	20674291
	VV-B 15C, KF 16	20674210
	VV-B 15C, KF 25	20674215
Coolant valve	VKW-B	20674220
Air admittance valve	VBM-B	20674217
Vacuum module for switching vacuum pump	VMS-B	20676030
...-I/O module	Digital... IN: 5-75 VDC / OUT: 60 VDC (2,5 A) IN: 5-50 VAC / OUT: 40 VAC (2,5 A)	20636228
	Analog... IN: 0-10 V / OUT: 0-10 V	20636229
	Analog... IN: 4-20 mA / OUT: 0-10 V	20635425
Level sensor	500 ml round bottom flask	20699908
Extension cable	VACUU·BUS® 2 m	20612552
	VACUU·BUS® 10 m	22618493
Y adapter	VACUU·BUS®	20636656



5 Operating and display elements

5.1 Operating elements




The operating elements are located on the controller front.
controller figure → see chapter 3.1 *Vacuum controller CVC 3000*

5.1.1 Selection knob


The selection knob of the controller is a combination of rotary knob and push-button.

	Selection knob	Meaning
Press selection knob		Press – Selection knob = <ul style="list-style-type: none"> ▶ Call up menu or function. ▶ Exit menu or function. ▶ Confirm and store setting or selection. ▶ Step to next menu, function or content. ▶ Call up Configuration menu while booting.
Turn selection knob		Turn – Selection knob = <ul style="list-style-type: none"> ▶ Select menu, navigation function. ▶ Value setting – increase/decrease. ▶ Adapt set vacuum (in mode Vac control).

5.1.2 Control panel

	Key	Meaning
Control panel keys		On/Off <ul style="list-style-type: none"> ▶ Switch on/off controller.
		Start/Stop <ul style="list-style-type: none"> ▶ Start/stop vacuum control. ▶ Confirm completed program when clock icon blinks. ▶ Confirm error and status indications.
		VENT – system venting; <ul style="list-style-type: none"> ▶ Keystroke < 2 sec = momentarily venting, control continues. ▶ Keystroke > 2 sec = venting to atmospheric pressure (max. 1050 mbar/787 Torr), control stops. ▶ Keystroke while venting = venting stops.

Control panel keys

	Mode – Select operation mode
	▶ With stopped operation: Mode menu for selecting the operation mode.
	Mode – Change function/mode
	▶ During running operation: To switch from <i>Pump down</i> to <i>Vac control</i> and further to <i>Auto mode</i> . ▶ During running operation: To switch between <i>Auto mode</i> and <i>Vac control</i> .

5.1.3 Key combinations








Menus and functions that are not intended for everyday use, can only be accessed through key combinations.

NOTICE

Wrong key combinations can lead to faulty settings.

⇒ First push and hold the key which must be hold and pressed, only then push the combination key shortly.

Key combinations (key shortcuts)


Combination	Meaning
 + 	Press and hold Selection knob + Press On/Off = Only when the controller is switched off ▶ Call up menu Language selection ▶ Call up menu Pressure unit
 + 	Press and hold VENT + Press On/Off = ▶ Call up menu Function
 + 	Press and hold Mode + press Selection knob = Only in Function menu ▶ Enable Vacuubus address assignment (frame marking). ▶ Confirm parameter transfer of selection Vario init.
	Press and hold Selection knob + turn it = ▶ Quick adaption set vacuum. (in mode Vac control) Only in combination with VARIO® ▶ Quick adaption motor speed high/low (in mode Pump down)

5.2 Display and user interface

After booting the pressure display appears, including **Bar graphic** and preset operation mode.

5.2.1 Pressure display

→ Example
Display after
switching on
CVC 3000

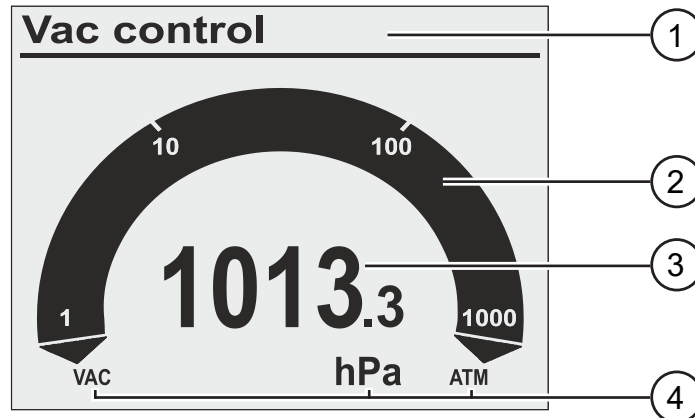

Meaning


1 Title bar (or status bar)	
Operation mode - Mode	<ul style="list-style-type: none"> ▶ Pump down ▶ Vac control ▶ Auto mode ▶ Program ▶ VACUULAN
Process time	<ul style="list-style-type: none"> ▶ hh:mm:ss (only displayed with running process)
2 Bar graphic	▶ Graphical display of actual pressure
3 Numerical value	▶ Actual pressure = digital pressure display
4 VAC	▶ Vacuum
mbar	▶ Pressure unit according to pre-setting (mbar, Torr, hPa)
ATM	▶ Atmospheric pressure

5.2.2 Display icons

When vacuum control has started additional icons appear on the display.







When starting operation

Display symbols during operation

Icon	Meaning
	Vacuum control is running (animation)
00:00:00	Process time; runtime vacuum control (hh:mm:ss)

Active component

Icons for active components









Icon	Meaning
	Pump is running; in combination with percentage sign = motor speed (only for VARIO systems)
	Venting* valve is active, i. e. open (VENT); Flashing cycle: continuous venting switched on.
	Coolant valve switched on, open
	In-line valve switched on, open
	Emission condenser (Peltronic) connected
	Level sensor activated (only when level sensor is connected)

* also named air admittance valve

The icon of a connected component is displayed as long as the component is running.




Status display while operation is running

Icons for control status

Icon	Meaning
	Pump down – continuous pumping
	Pump down: lower pressure limit reached VACUU·LAN: pump down to set pressure Vac control: for 2-point control – pump down to set pressure
	VACUU·LAN: pressure increase to switch on pressure Vac control: preset maximum exceeded
	VARIO control: pump down to set point. Auto mode: pump down and boiling point detection within the preset time interval regarding changing process conditions.
	VARIO control: reaches and tracks boiling point. The next program step starts when the programmed pressure has been reached or the preset time has elapsed.
	2-point control: pressure in hysteresis, pump switched on
	2-point control: pressure in hysteresis, pump switched off
	Turbo mode switched on (for VARIO [®] pump in combination with turbomolecular pump)

Additional information


Information icons

Icon	Meaning
	Clock - Program completed* - Mode VACUU·LAN: delay time elapses
	Lock – operation locked
HI	HI mode for Pump down = optimum speed for the respective pressure.
..%	Percentage value for Pump down motor speed.
100 	Set value for Vac control.

* The clock icon keeps flashing until the **Start/Stop** button has been pressed to acknowledge the end of program.



Fault indication (warning symbol)

Error display

Icon	Meaning
	Flashing: warning!

When device connected to SUB-D (Option)

Active connection to RS232 port





Icon	Meaning
	Controller in remote mode; controller only controllable via connected PC or Notebook, local operation disabled.
	VACUU·CONTROL [®] -adapter connected; Remote and local operation possible. → Remote operation via end device (e. g., PC, Smartphone).

5.2.3 Signal sounds (warning beep)

Setting **Sound On** in menu **Configuration/Display** is required to hear the audio signals.

Meaning audio signal

Audio signal (beep)

Audio signal	Meaning
1x  	Short beep for each keystroke.
2x  	Audio warning for error indication. In short intervals a number of warning beeps are to be heard. This Audio warning is active until error clearance or reset.



Error messages are indicated by differing numbers of beeps (audio warning).


For the list of possible warning beeps
→ see chapter **8.1 Error display**.

5.2.4 Menu display in general

The controller includes several menus and submenus, e. g., **Configuration**, **Function**, **Display...**

Submenu

→ Example
Submenu
Configuration

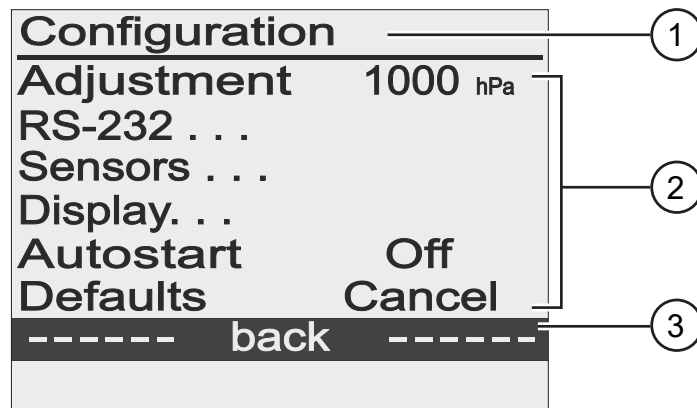

Meaning

1 Titel bar	▶ Menu name
2 Menu interface	▶ Selectable functions or submenus (on the right side of the display) ▶ Adaptable value or ▶ selectable content
3 Back (return)	▶ Call-up previous menu or ▶ previous display



For detailed descriptions about individual menus,
→ see chapter **7.1 Operation menus**.

5.3 Handling CVC 3000


Handling and Operation

The handling of the controller is menu-driven. Menus are accessed via push buttons on the control panel or via key combinations. Use the selection knob to select function or menu.

Operating steps and actions are displayed by an illustration, which is complemented by action symbols.

→ see chapter **1.2.2 Symbols and icons**.

Navigation

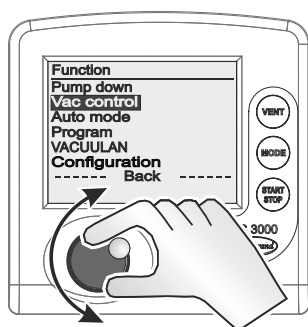

Turn selection knob to select a menu by shifting the bar marking.


→ **bar marking** up/down.

Submenus




Submenus are highlighted with points.

Selection

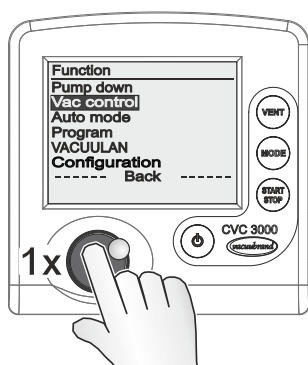

Press selection knob to confirm selection.

Input (data entry)

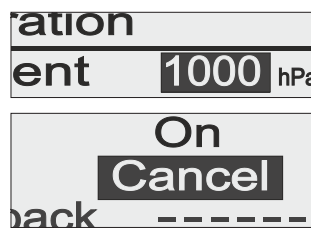


Changeable values are positioned on the right side in the display.

Text on the right side accords to content selection like in a drop down list.


Exception: menu **Program**, in this menu data and value are editable.

Example: enable entry and edit

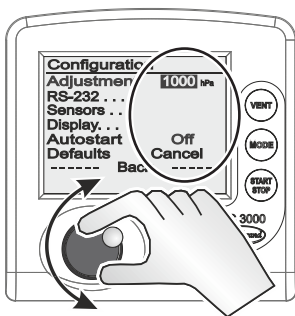

1. Select the required line and press selection knob.
 - ☒ Marking jumps to the input field.
 - ☒ Input/Content selection enabled.
2. Turn the selection knob.
 - ☒ Value/Content changes.
3. Adapt the numeric value within the specified min./max. range or select the required function out of the available content.
4. Confirm input/selection by pressing the selection knob.
 - ☒ Value is stored or
 - ☒ selected function starts.

Back (return)

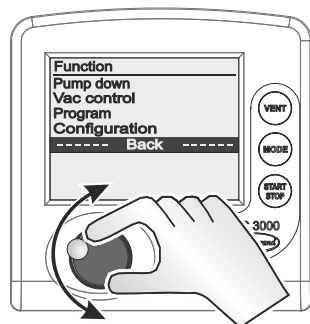

Place the bar marking on line **back** and press the selection knob to return to previous menu, display or to pressure display.




In submenu **Sensors** the display returns to previous menu only after the selection of a sensor.

6 Operation

6.1 Switch-on/-off controller

Switch-on

Switch-on CVC 3000

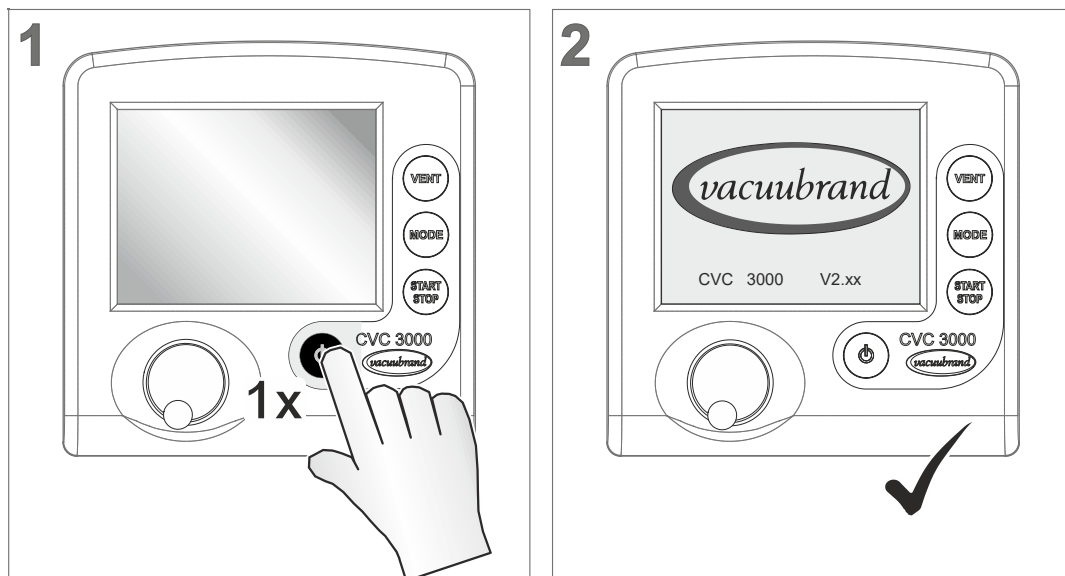

- ☒ Initial screen: company logo and firmware version, for approximately 2 seconds.
- ☒ Pressure graphic is displayed.

Switch-off


Switch-off CVC 3000

⇒ Press key **On/Off**

- ☒ Controller switched off (display off).

6.2 Select language and pressure unit

Select language and pressure unit

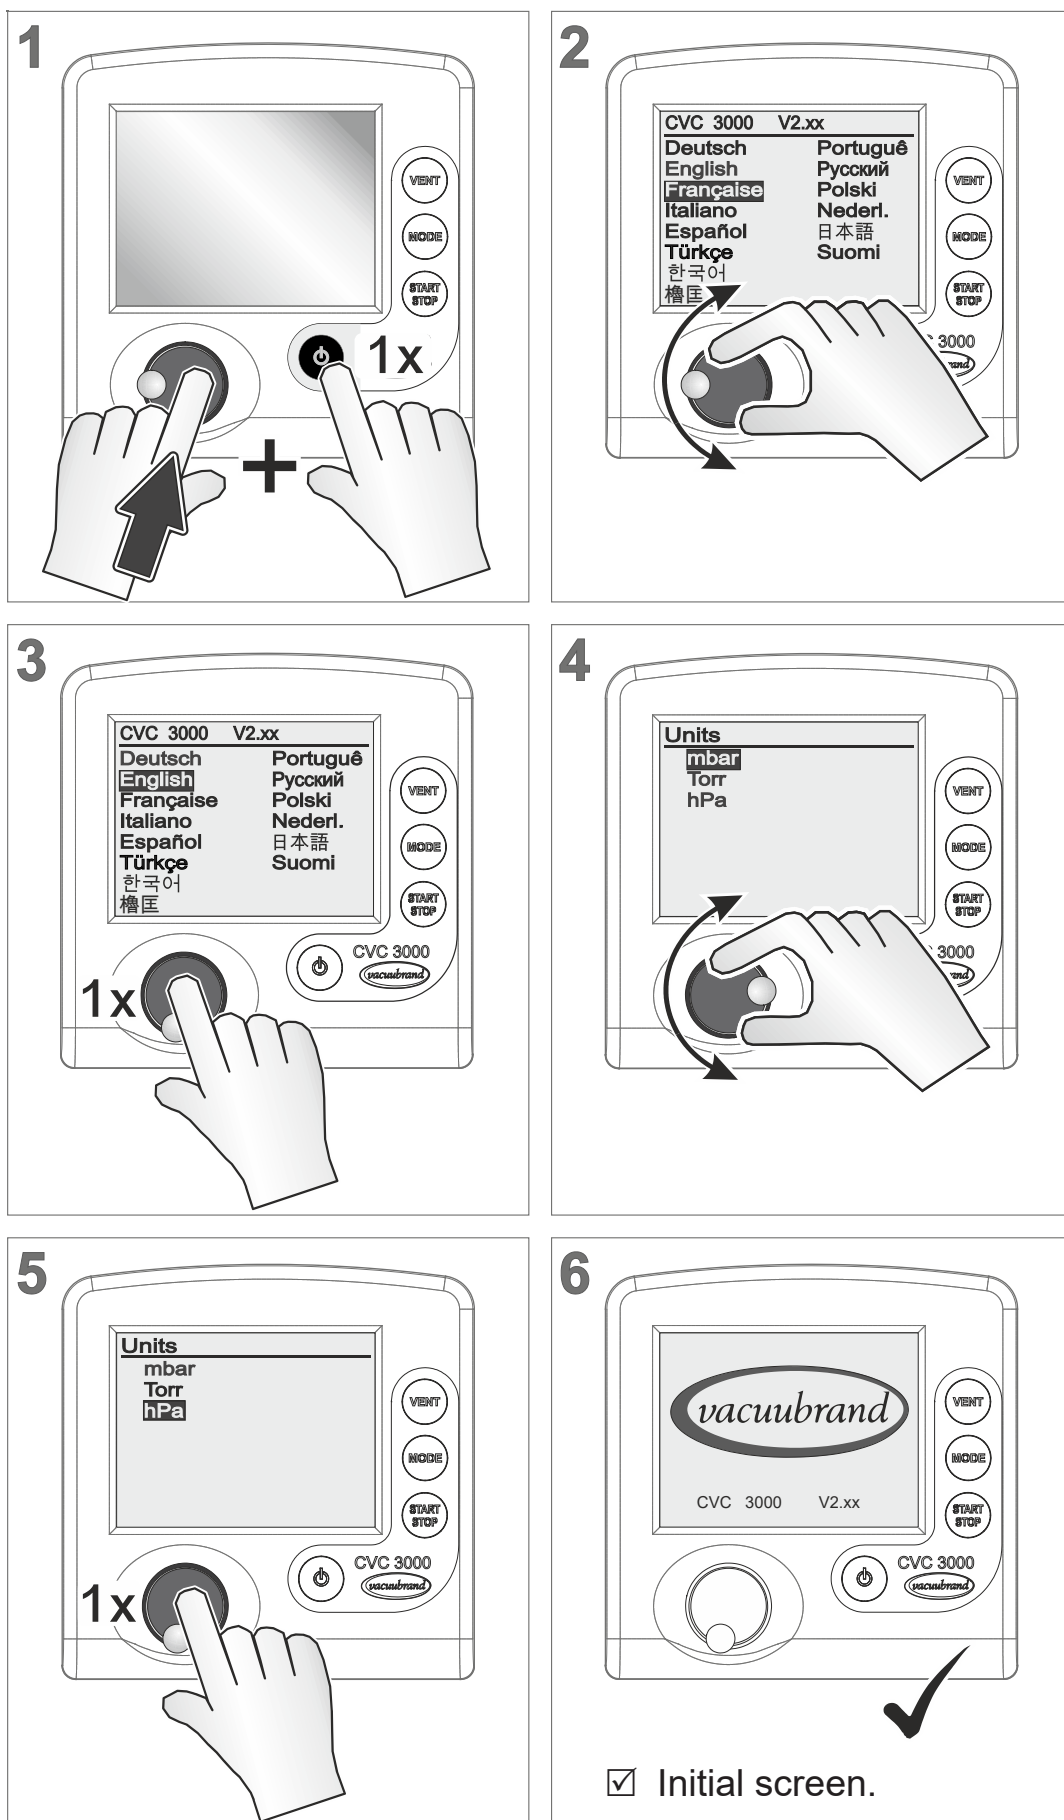


6.3 Mode – Operation mode



The controller is supplied with several operating modes. Only when the controlling process is stopped it is possible to select an operation mode.

6.3.1 Select operation mode

→ Example
Call-up mode menu

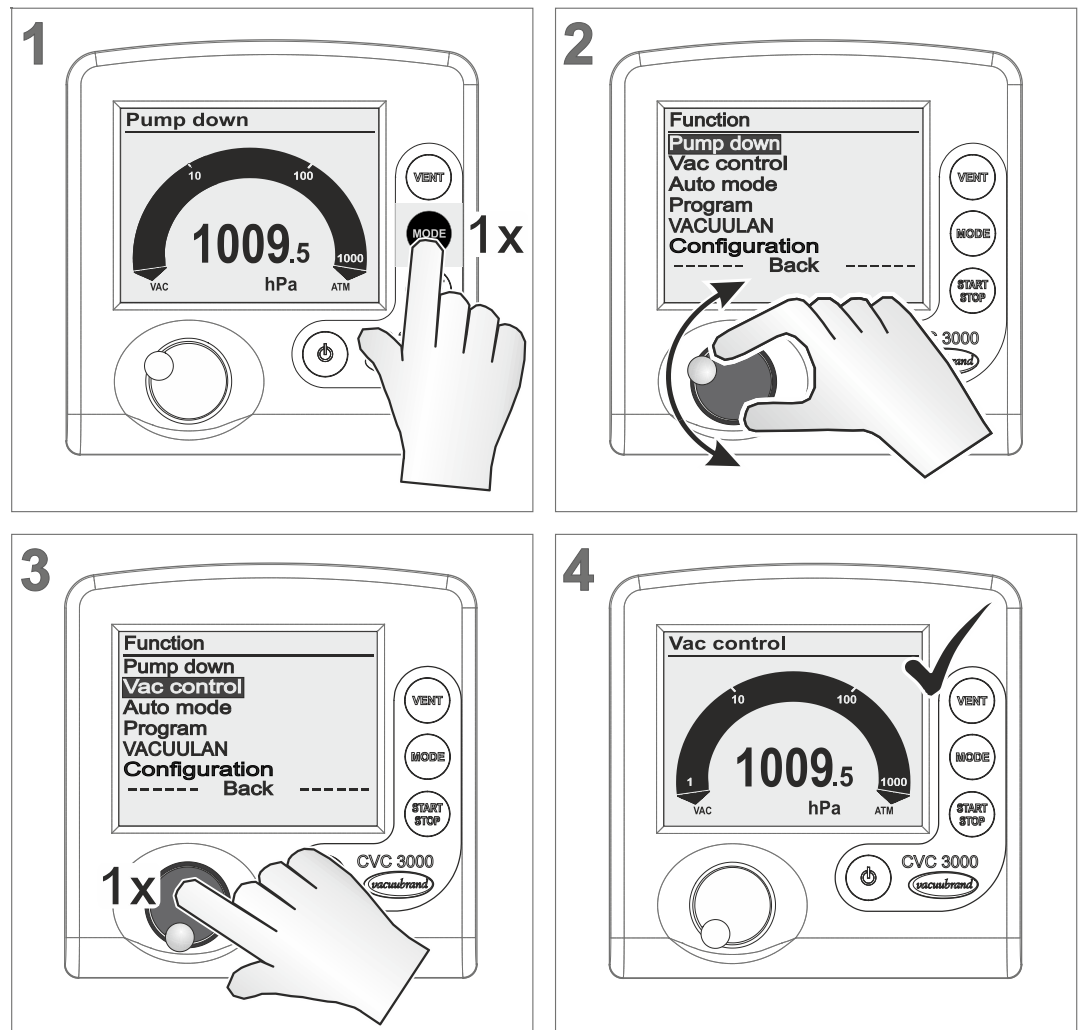

☑ Title bar shows the selected operation mode (**Mode**).




Select any other operation mode in the same way as described above for **Vac control**.

After 20 seconds without action, the display will return automatically to pressure display.

6.3.2 Mode menu

Mode menu display

→ Example
Menu description

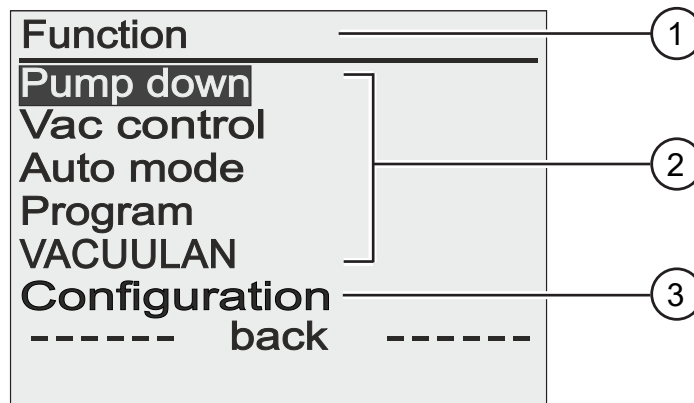

Meaning and
operation modes

1 Title bar menu name

2 Selectable operation modes

Pump down

- ▶ Continuous pump down or
- ▶ pump down with pressure and time presetting.
- ▶ **VARIO®**: Pump down with adjustable motor speed (pumping speed) and continuous speed control.

Vac control

- ▶ Control to a preset vacuum value.

Auto mode

- ▶ Controlling a **VARIO®** pump in **Auto mode**: Detect and track boiling point automatically, exact vacuum adaption even with flexible process conditions.

*Listed only with **VARIO®** pump.*

Program

- ▶ Load, edit and/or store program.
- ▶ max. 10 programs with pressure and time presetting.

VACUULAN

- ▶ Control of the vacuum pump according to demand, optimized for vacuum networks.

*Listed only with **VARIO®** pump or **VMS** module, e. g., for pump control.*

3 Menu Configuration

⇒ Select the mode suitable for vacuum apparatus and planned process.


6.4 Start controlling

START
STOP

Start vacuum controlling after selecting the required operation mode. The controller works in delivery status with the default settings of the factory setting.

Start controlling

→ Example
Start CVC 3000

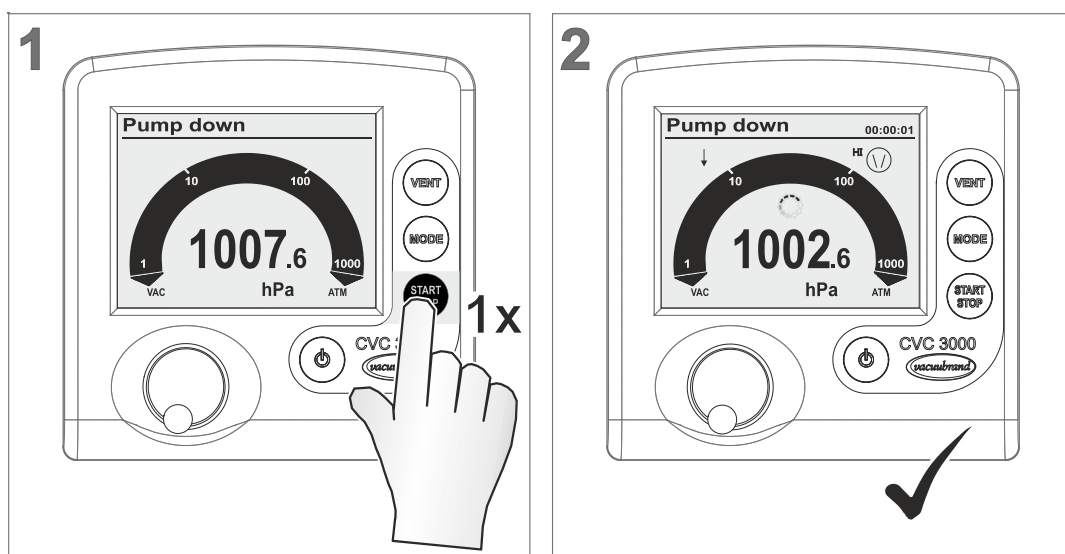

- ☒ Controller starts.
- ☒ Icons are displayed.

6.5 Control during operation

6.5.1 Venting (VENT)



DANGER

Danger of explosion when venting with air by forming of explosive mixtures.

Depending on the process venting can cause formation explosive mixtures.

- ⇒ Never vent processes with air which can form explosive mixtures.
- ⇒ If necessary vent with inert gas (max. 1.2 bar absolute).

IMPORTANT!

Certain processes may cause overpressure.


VENT

Venting

The **VENT** button is used to vent the system. A short click on this button will momentarily vent the system as the process continues. Holding the **VENT** key for longer than 2 seconds will cause the system to be vented to atmospheric pressure and the pump will stop running; max. 1060 mbar (795 Torr). Continuous venting stops when pressing **VENT** key again.

Momentarily venting


→ Example
Momentarily venting

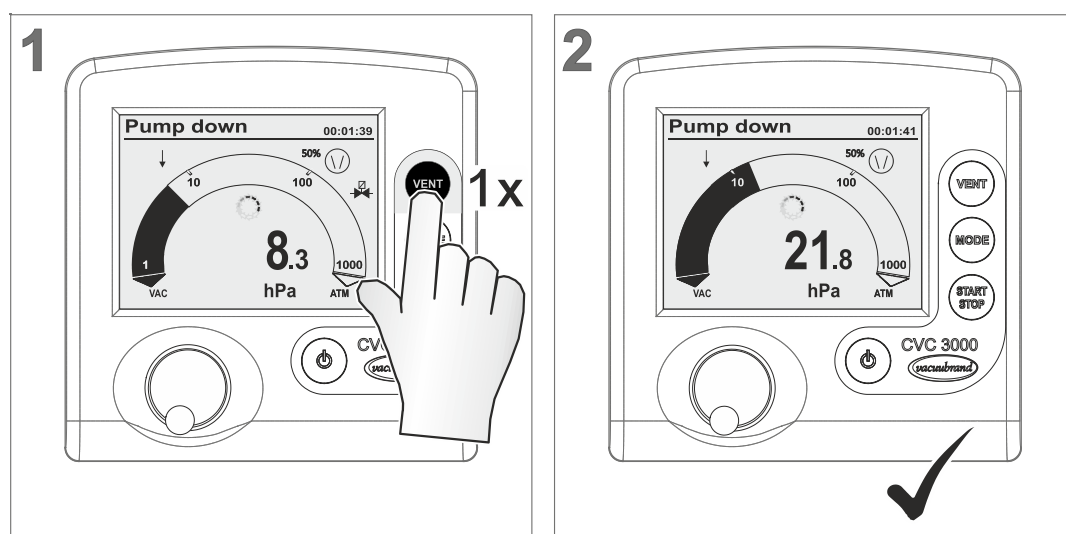

- ☑ Venting impulse, venting valve respectively air admittance valve opens momentarily → short-term pressure increase.

Continuous venting

→ Example
Continuous venting

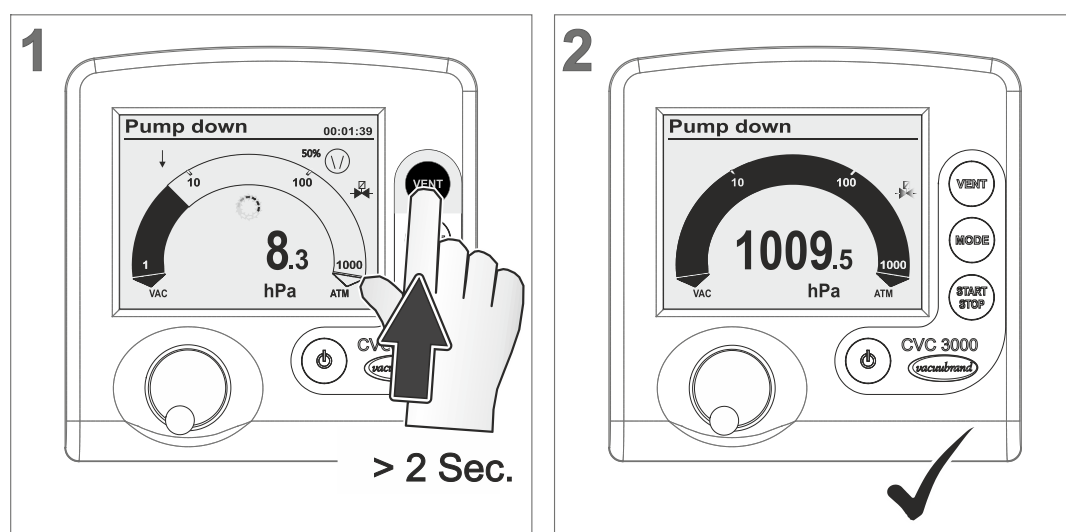

- ☑ Icon for venting valve is flashing,
- ☑ Venting valve opens → continuous pressure increase until atmospheric pressure → venting valve closes.
- ☑ Controller stops.

6.5.2 Change operation mode




During running operation the operation mode can be switched between *Pump down*, *Vac control* and *Auto mode*¹ by pressing **Mode** key.

Switch mode during running operation


→ Examples
Switch mode

Pump down
↓
Vac control

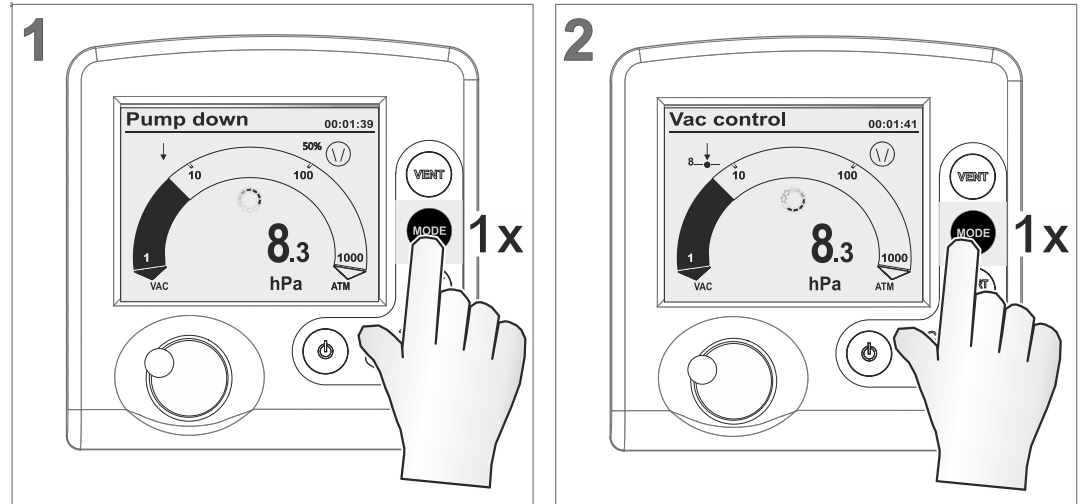

☑ Operation mode switched to *Vac control*.

↓
Auto mode
↓
Vac control
with **VARIO®**

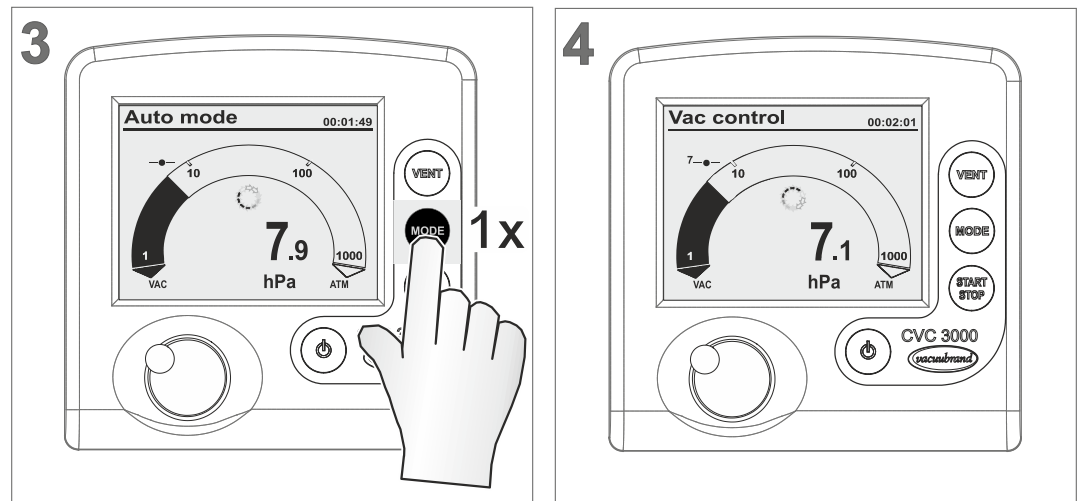


☑ Operation mode switched from *Vac control* to *Auto mode*¹ and back.

☑ Set vacuum adopted from last status in *Auto mode*¹.

¹ -> Only when connected to **VARIO®** pump.

Switch back from **Vac control** to **Pump down**.

Switch back to primary mode

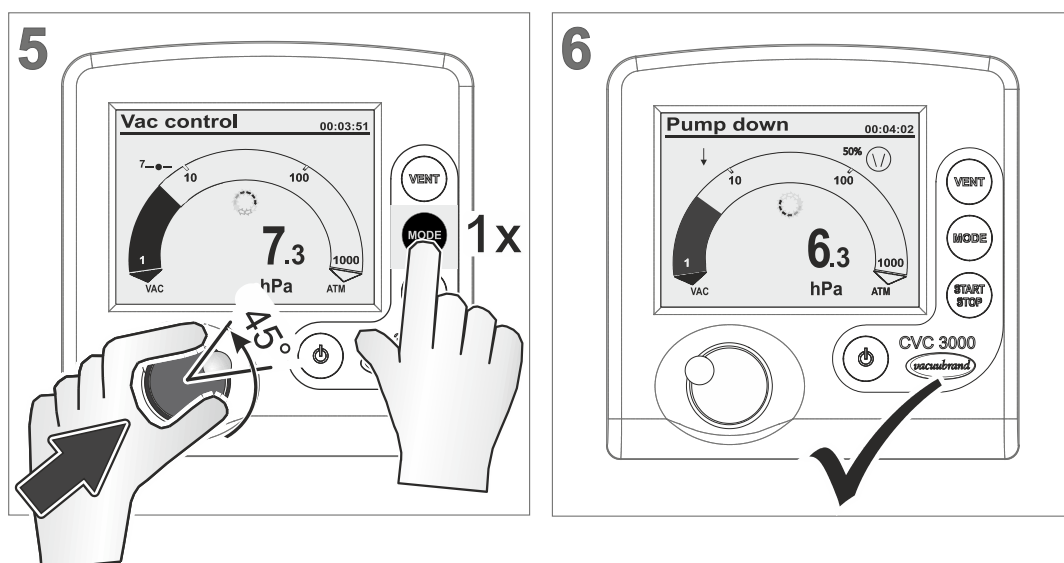

☑ Title bar displays **Pump down**.

Typical applications

Pump down → **Vac control**:

Semiautomatic distillation. Recommended for applications for which the process vacuum is still to be determined. Firstly the vacuum pump is pumping down rapidly in mode **Pump down**. As soon as the required process vacuum has been reached, e. g., boiling vacuum, this vacuum can be maintained by switching to **Vac control**. The actual pressure is adopted as the required set vacuum.

Auto mode ⇌ **Vac control**:

With a connected **VARIO®** pump a controller working in **Auto mode** will detect and track the boiling point automatically. The vacuum will be adapted continuously to the process.

If a particular process vacuum is required, the mode can be switched back again to **Vac control**.



Switching the mode during operation via **Mode** key works only temporarily. After stopping the controller switches back to its primary mode.

6.5.3 Display graphic (curve)


Pressure history

In addition to the bar graphic of the pressure display the display can be switched to a diagram named **Graphic** which shows a pressure vs. time curve.

That **Graphic** curve will only be displayed while operation is running. With each start the recording restarts.

Call up graphic

→ Example
Call up pressure
history display

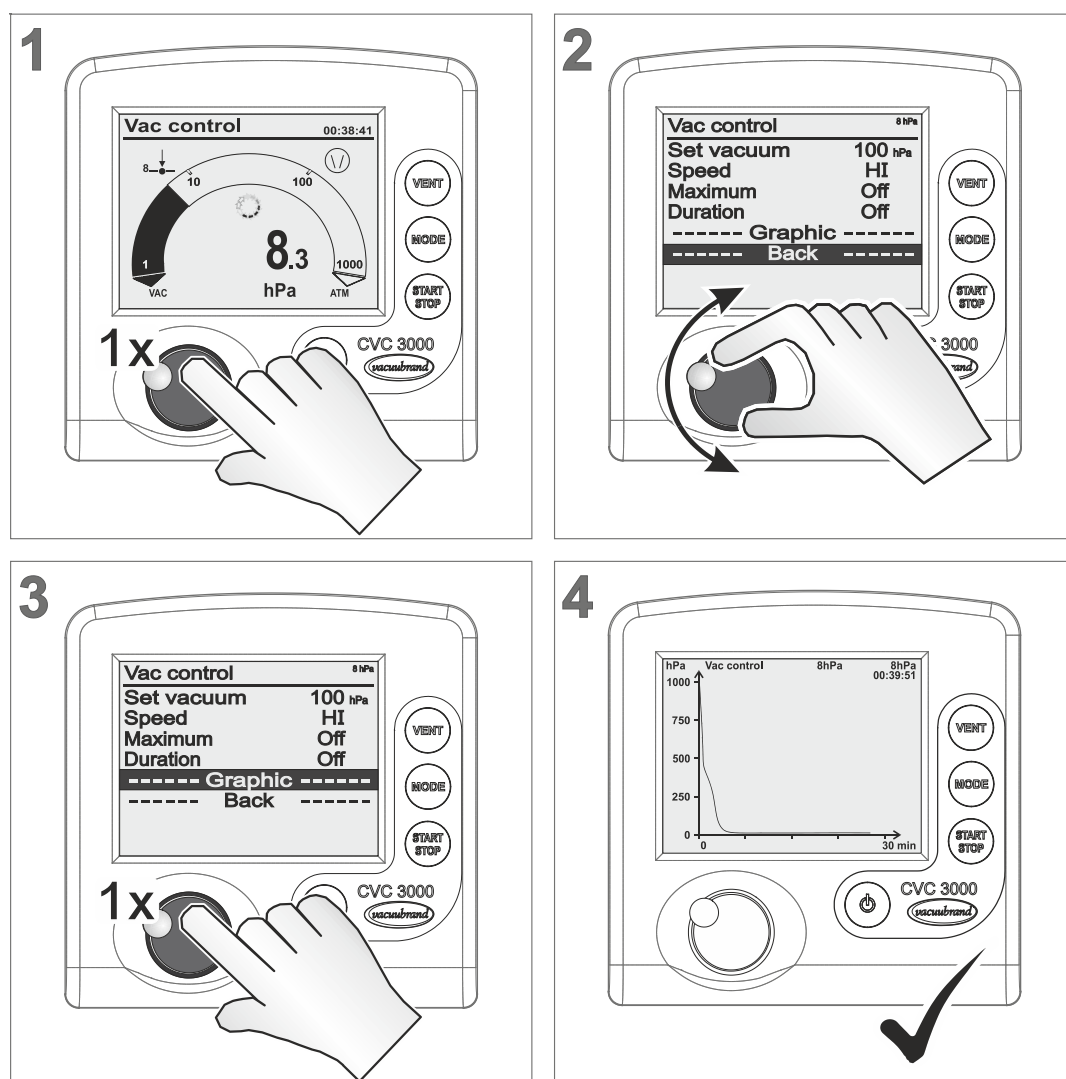


- ✓ **Graphic** menu is displayed with the pressure curve of the actual process.



To call up **Graphic** with pressure history for other operation modes, do like described above.

Graphic menu

Description pressure
history display

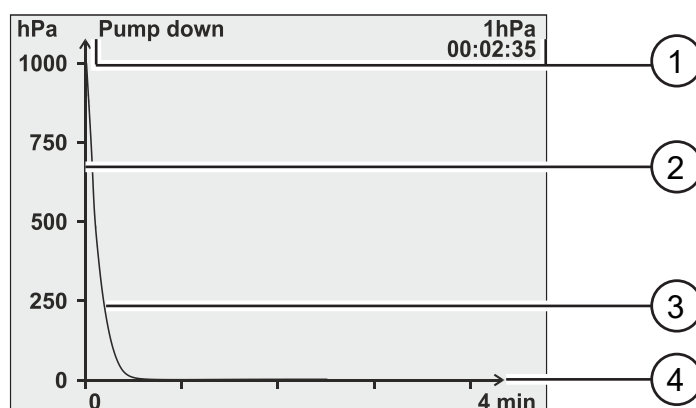


Meaning

- 1 Header**
 - ▶ Active operation mode.
 - ▶ Vacuum set point; for *Vac control* or *Auto mode*.
 - ▶ Actual vacuum value (actual pressure).
 - ▶ Elapsed process time.
- 2 Axis – pressure**
 - ▶ Unit according to pre-settings (mbar, Torr, hPa).
- 3 Pressure graph**
 - ▶ Pressure/time progress.
- 4 Axis – time**
 - ▶ Continuous, automatically scaling time (minute, hour).

6.5.4 Quit display graphic

Return to pressure display

→ Example
Switch back to
basic display

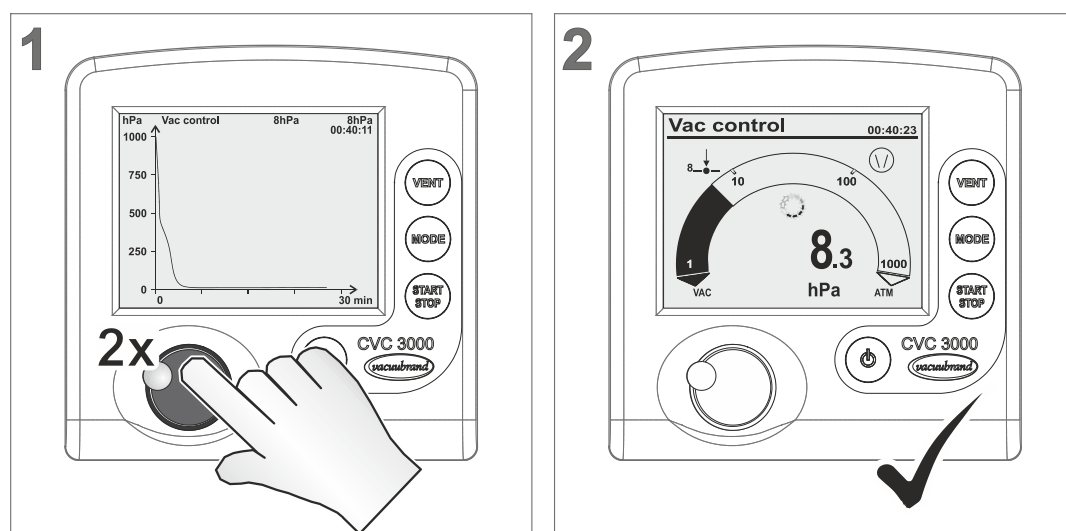

☒ View basic display.

6.6 Quick adaption during operation


6.6.1 Set vacuum

In mode **Vac control** the set vacuum can be adapted directly during running operation.

Adapt set vacuum → fine tuning

1 detent = 1 pressure value (mbar, Torr, hPa)


→ Example
Adapt set vacuum
fine tuning

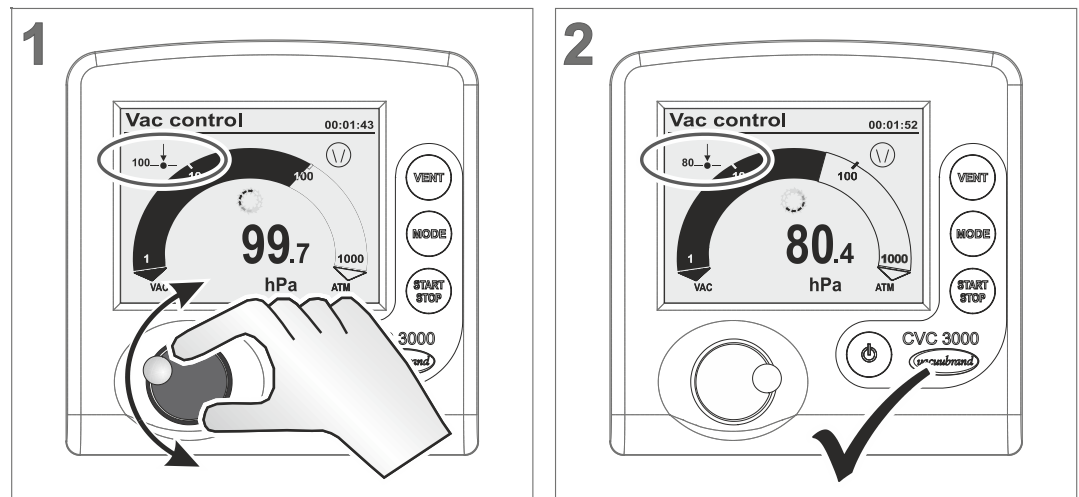

☑ Controller controls to new set vacuum.

Adapt set vacuum → quick tuning

→ Example
Adapt set vacuum
quick tuning

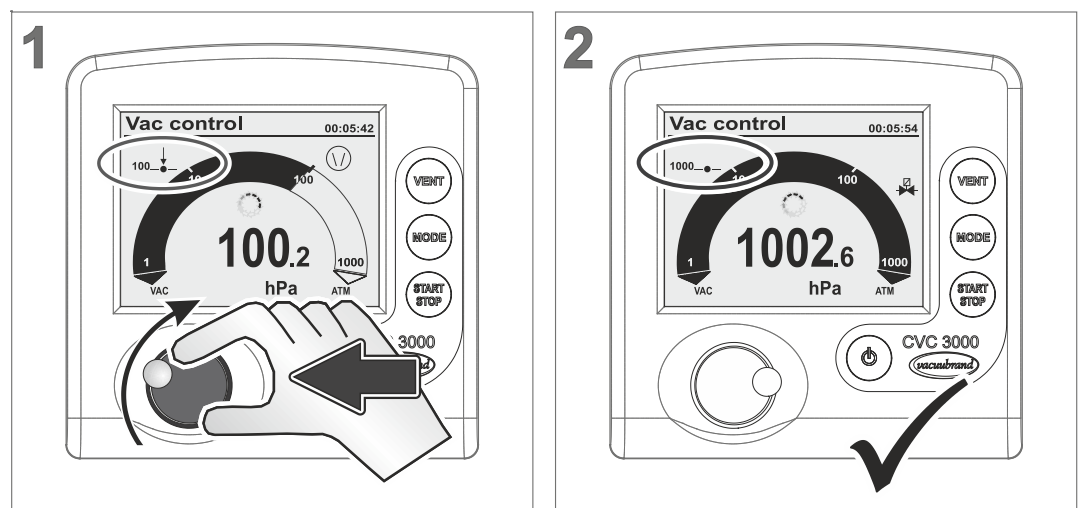

⇒ Press selection knob and turn it clockwise: increase set vacuum (venting).

⇒ Press selection knob and turn it counterclockwise: decrease set vacuum (vacuum pump on).


☑ Controller controls to the new set vacuum which is displayed while releasing the selection knob.

6.6.2 Motor speed (only VARIO®)

In mode **Pump down** the motor speed of a **VARIO®** pump can be adjusted directly during running operation.

Pump down – adjust motor speed

→ Example
How to change
motor speed

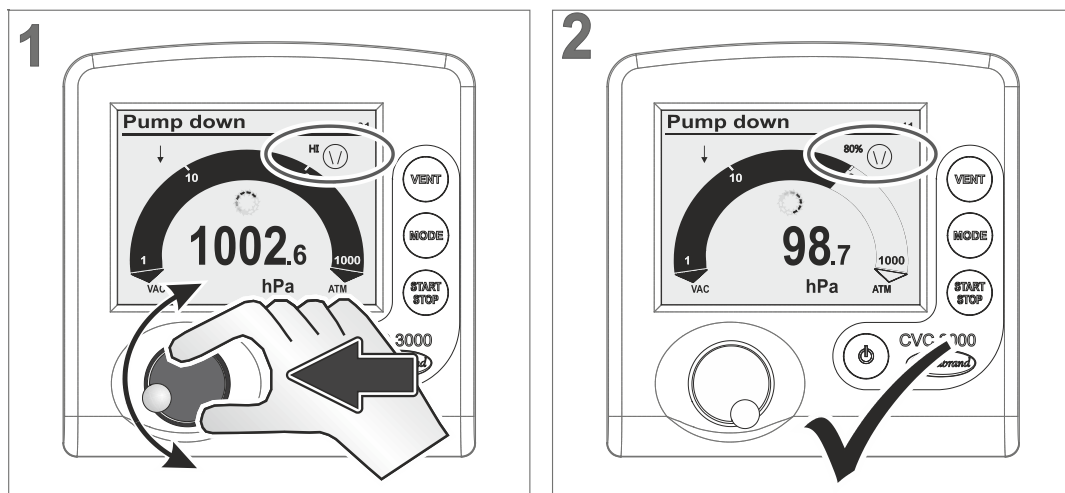


- ✓ Pump icon with percentage value.
- ✓ **VARIO®** pump runs with adjusted motor speed.

6.7 Stop control

Stop control

→ Example
Stop CVC 3000

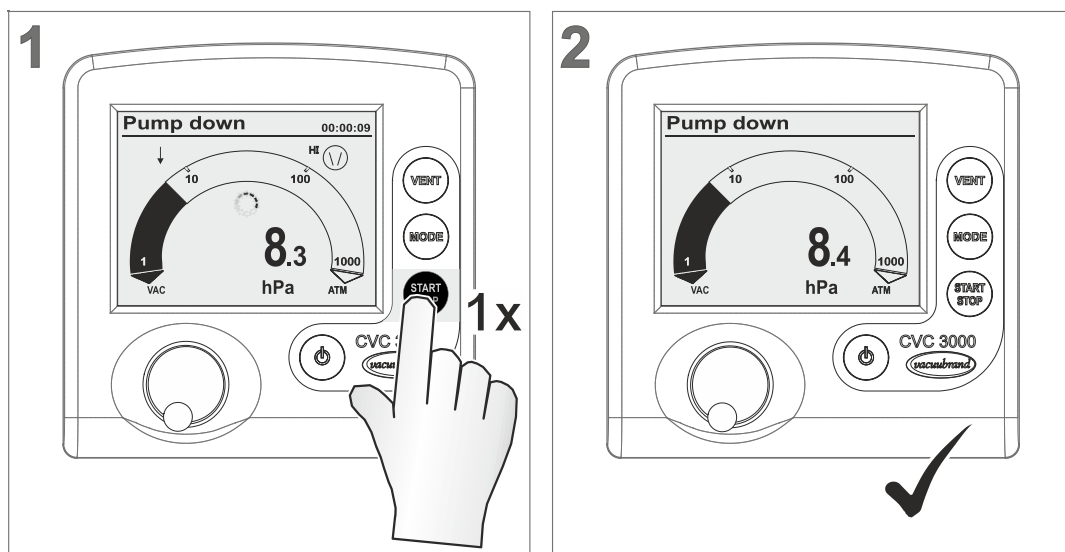

- ✓ Controller and vacuum control stops.
- ✓ Display icons switched off.

7 Advanced menus and operation

7.1 Operation menus


Optimizing operation
mode

A selected operation mode can be adapted and optimized for the process through the corresponding operation menu. The settings in an operation menu include mainly: motor speed, set vacuum or time presets. Settings in operation menus are retained also after switching on/off.

Menu **Program** is for storing up to 10 individual programs, e. g., to store control settings for frequently repeated processes.

Call up submenu of an individual operation mode

→ Example
Call up operation
menu

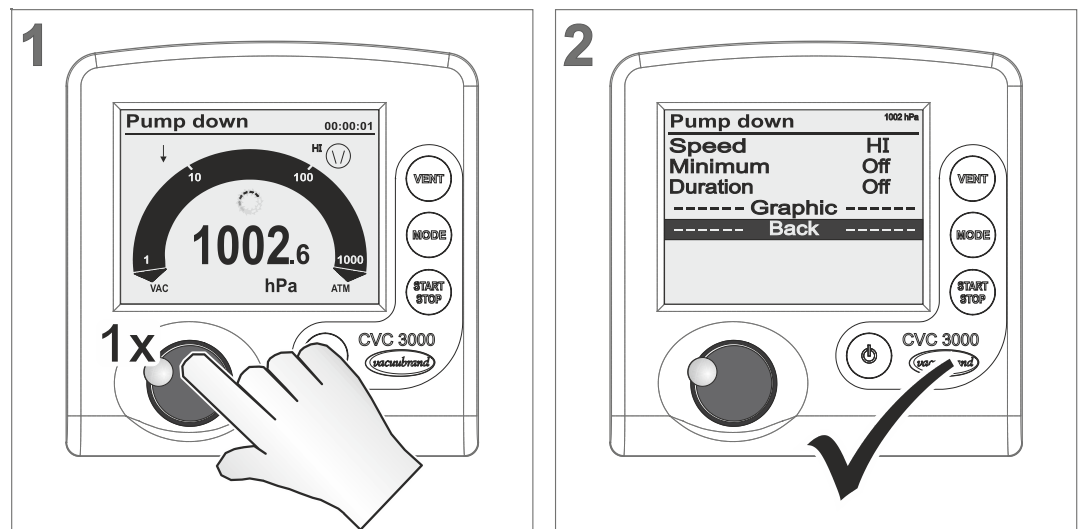

- ☒ Corresponding menu of the preset operation mode is displayed.

To call up an operation menu, press the selection knob. Adaptations are possible during a running process as well as when control is stopped.



Use operation menu to optimize vacuum control for application requirements.

7.1.1 Pump down

Meaning Continuous pump down with pressure and time presets.

Menu – Pump down

→ Example
Operation menu
Pump down

Pump down		1013 hPa
Speed	HI	
Minimum	Off	
Duration	Off	
----- Graphic -----		
----- Back -----		

Parameter
Pump down

Parameter	Meaning
Speed (%)	VARIO® : Speed settings for pump down. Adjustment range: 1–100; HI*
Minimum** (mbar, Torr, hPa)	Vacuum set point; once reached, the controller switches off the vacuum pump or closes the in-line valve. Adjustment range: Off; 1–1060
Duration** (Min)	Presetting process runtime from Start on. Adjustment range: Off; 1–1440
Delay (Min)	Delay time for an optional coolant valve. Adjustment range: Off; 1–300

* HI mode: optimum speed for the respective pressure.

** If **Minimum** and **Duration** are set to **OFF**, pump down has to be stopped by pressing START/STOP key.

Application example – cabinet dryer

Application example
for Pump down

Set **Minimum** to a vacuum value below boiling pressure and the controller will switch the vacuum pump off, once the liquid has completely evaporated.

7.1.2 Vac control

Meaning Control to a set vacuum value.

Menu – Vac control

→ Example
Operation menu
Vac control

Vac control		1002 hPa
Set vacuum	100	hPa
Speed	HI	
Maximum	Off	
Duration	Off	
----- Graphic -----		
----- Back -----		

Parameter
Vac control

Parameter	Meaning
Set vacuum (mbar)	Setting for lower vacuum level for 2-point control or precisely for VARIO ® pump. Adjustment range: Turbo*; 1–1060
Speed (%)	VARIO ®: Speed settings for pump down. Adjustment range: 1–100; HI**
Hysteresis*** (mbar, Torr, hPa)	Only for VMS or in-line valve with vacuum pump: control range for 2-point control. Adjustment range: Auto; 1–300
Maximum (mbar, Torr, hPa)	Setting for upper vacuum level. Once reached, control switches off. Adjustment range: Off; 1–1060
Duration (Min)	Presetting process runtime from Start on. Adjustment range: Off; 1–1440
Delay (Min)	Delay time for an optional coolant valve. Adjustment range: Off; 1–300

* Turbo mode: auto-adapting vacuum control for best ultimate vacuum.
Best backing pressure for operation with a turbomolecular pump.

** HI mode: optimum speed for the respective pressure.

*** VARIO pumps work without hysteresis.

Application example – filtration

Application example
for Vac control

Set the set vacuum higher than the boiling pressure of the liquid and set **Maximum** value even a little bit higher. If the filter runs dry or if the filter is fractured, the pressure will increase and the control will be stopped automatically.

Hysteresis values Auto

Factory settings
Hysteresis

Set vacuum (mbar)	5	10	50	80	100	200	500	700	900	1000
Hysteresis (mbar)	2	2	5	8	9	17	40	55	71	78

7.1.3 Auto mode (only valid for VARIO® pump)

Meaning Automatic detection and tracking of boiling point, unaffected by varying process conditions.

Menu – Auto mode

→ Example
Operation menu
Auto mode

Auto mode 999 hPa	
Sensitivity	Normal
Speed	HI
Minimum	Off
Duration	Off
----- Graphic -----	
----- Back -----	

Parameter
Auto mode

Parameter	Meaning
Sensitivity	Setting affects processing speed: Low Fast; large amounts of uncritical solvents Normal Normal; basic setting for almost all distillations High Slow; small amounts, for solvents with tendency to foam
Speed (%)	VARIO® : Motor speed limitation during tracking. Adjustment range: 1–100; HI*
Minimum (mbar, Torr, hPa)	VARIO® : Vacuum setting; once reached, controller stops the VARIO® pump. Adjustment range: Off; Auto**; 2–1060
Duration (Min)	Presetting process runtime from Start on. Adjustment range: Off; 1–1440
Delay (Min)	Delay time for an optional coolant valve. Adjustment range: Off; 1–300

* HI mode: optimum speed for the respective pressure, recommended setting.

** Complete solvent evaporation will be detected and the process will then be stopped.

Application example – rotary evaporator

Application example
for Auto mode

Use **Minimum** to prevent rotary evaporator from receiving re-evaporation from the flask. Set **Minimum** value to the vapor pressure of the solvent at ambient temperature.

7.1.4 Program

Meaning

Up to 10 individual programs including vacuum and time presettings can be loaded, edited, and stored.

Menu – **Program**

→ Example
Operation menu
Program

Program 0		1010 hPa
Edit		
Open		0
Store		0
----- Graphic -----		
----- Back -----		

Parameter Program

Parameter	Meaning
Edit	Edit program with presettings for a process cycle or edit an existing program.
Open	Load the selected program.
Store	Store the program under the selected number. (memory capacity for up to 10 programs)
Hysteresis (mbar, Torr, hPa)	Only for VMS or in-line valve with vacuum pump: control range for 2-point control. Adjustment range: Auto; 1–300
Delay	Delay time for an optional coolant valve. Adjustment range: Off; 1–300

Hysteresis values Auto

Factory settings for
Hysteresis

Set vacuum (mbar)	5	10	50	80	100	200	500	700	900	1000
Hysteresis (mbar)	2	2	5	8	9	17	40	55	71	78

For further descriptions of program functions
→ see chapter **7.2 Program functions**.

7.1.5 VACUULAN

Meaning Vacuum control, optimized for **VACUU-LAN®** vacuum networks by VACUUBRAND.

Menu **VACUULAN**

→ Example
VACUULAN display

VACUULAN		1008 hPa
Set vacuum	25	hPa
Switch on	200	hPa
Delay	15	min
----- Graphic -----		
----- Back -----		

Parameter
VACUULAN

Parameter	Meaning
Set vacuum (mbar)	Setting for lower vacuum level, which shall be reached easily when the vacuum network is not used. Adjustment range: 1–1060
Switch on (mbar, Torr, hPa)	Limit for pressure increase. If pressure exceeds this limit, the pump will begin to pump down. Adjustment range: 26–1060
Delay (Min)	Delay time for an optional coolant valve after reaching set vacuum. Adjustment range: Off; 1–300


7.2 Program functions


Meaning In menu **Program** presets for up to 10 different application scenarios can be stored.

Use **Program** for frequently used applications.

7.2.1 Open/Change program

→ Example
Open Program 2

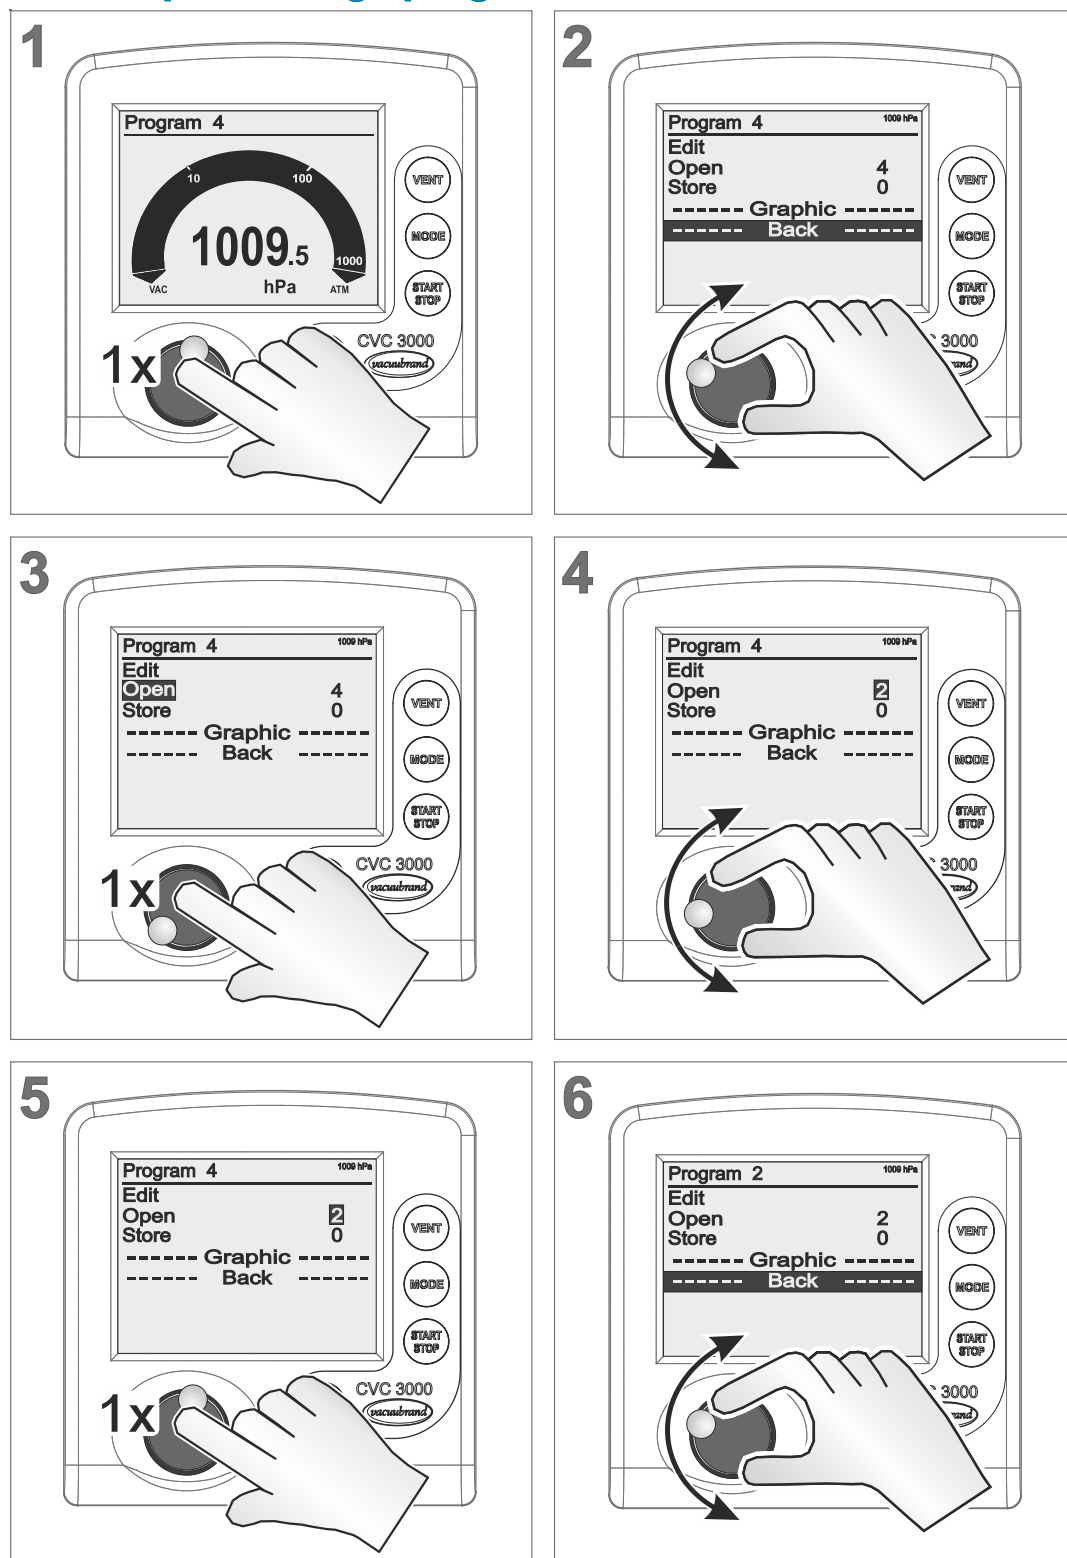

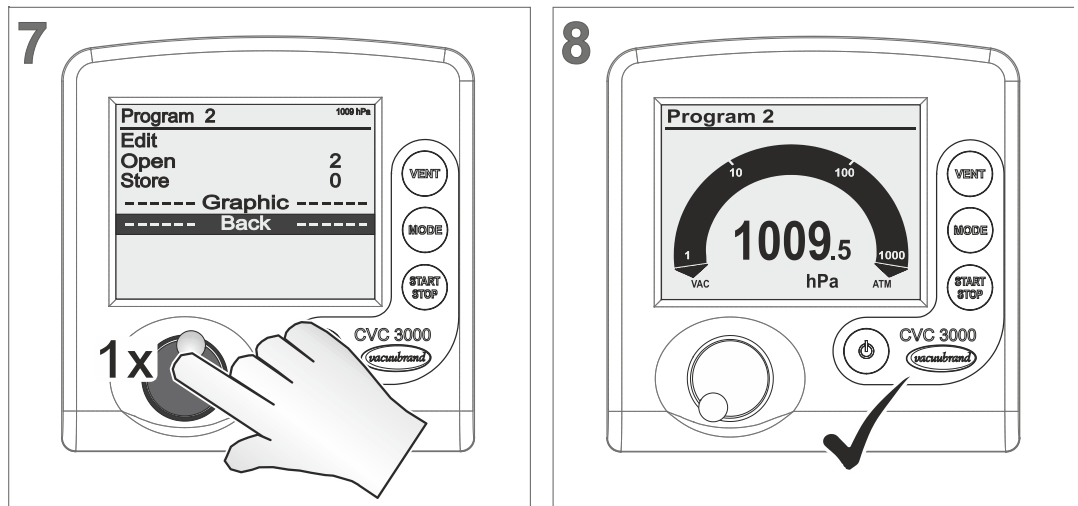


- ☒ Controller is running with settings of program 2.
- ☒ Program 2 displayed in title bar.

7.2.2 Edit program

Open program editor

→ Example
Call up program
editor

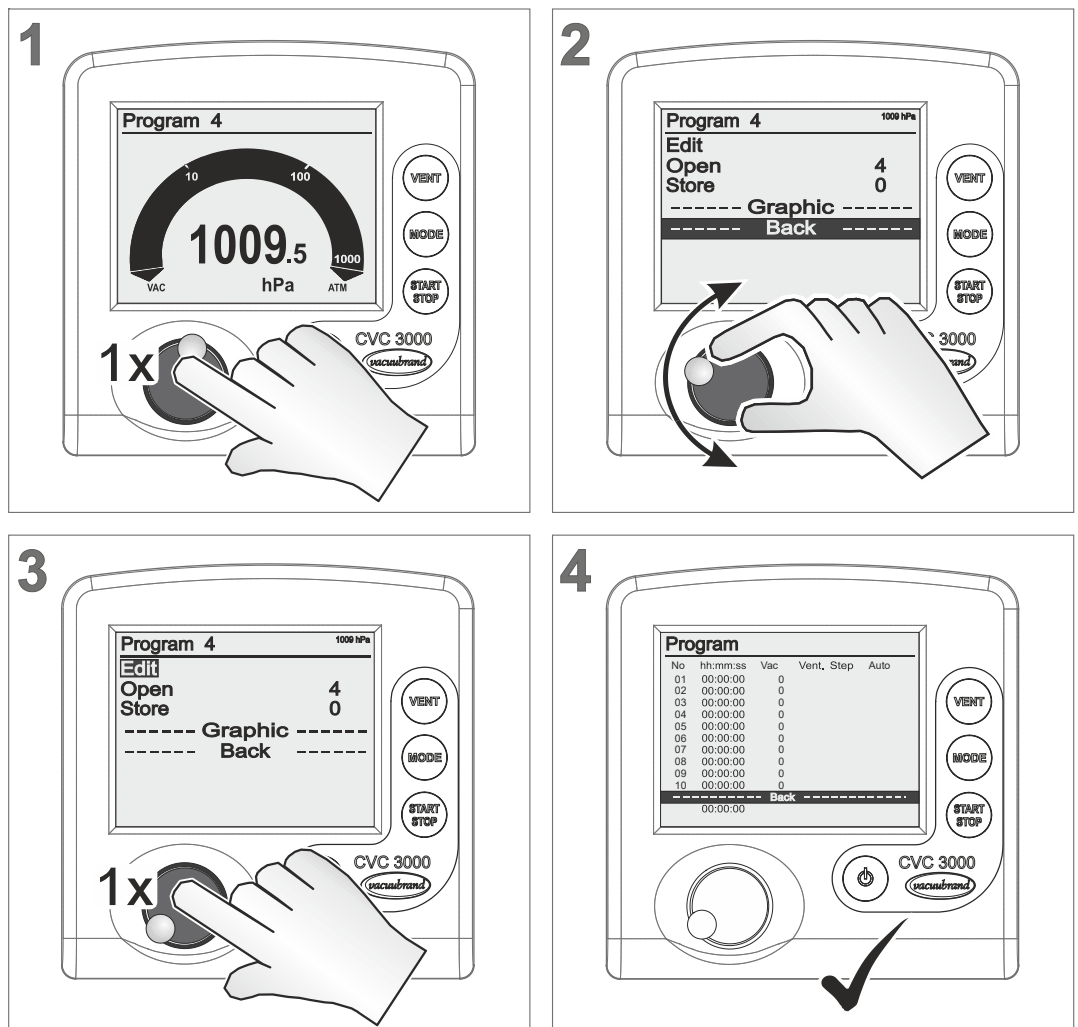

Explanation program editor

→ Example
Menu explanation

Program					
No	hh:mm:ss	Vac	Vent.	Step	Auto
01	00:00:00	ATM	✓	✓	
02	00:05:00	10			
03	00:10:00	10			
04	00:01:00	500	✓		
05	00:09:00	500	✓		
06	00:10:00	5			
07	00:20:00	5			
08	00:01:00	ATM	✓	✓	
09	00:00:00	0			
10	00:00:00	0			
----- back -----					
00:56:00					

1 Title bar menu name

2 No

► Number 1–10, sequence of program steps.

hh:mm:ss

Timer for individual program steps:

- Until vacuum value has been reached.
- Hold vacuum level.

Vac

► Preset a vacuum level.

Vent.

► Controller includes venting valve for control.

Step

- Reach vacuum level as quickly as possible.
- Timer starts after vacuum level has been reached.

Auto (displayed only in combination with **VARIO®**).

► Detect and track boiling point.



3 Program steps

Up to 10 program steps can be edited individually.

4 Total runtime

Total amount of time of individual program steps.

Adjustable parametersAdjustable program
step parameters

hh:mm:ss	00:00:00–99:59:59			
Vac	0–1060; ATM		(Torr: 0–795; ATM)	
	ATM = atmosphere; this starting point is always attainable.			
Vent.	<input type="checkbox"/>	Off	<input checked="" type="checkbox"/>	On
Step*	<input type="checkbox"/>	Off	<input checked="" type="checkbox"/>	On
Auto*	<input type="checkbox"/>	Off		Pump down and boiling point detection within the preset time interval regarding changing process conditions.
	<input type="checkbox"/>	Off		Reaches and tracks boiling point. The next program step starts when the programmed pressure has been reached or the preset time has elapsed.

* either selection **Step** or **Auto** possible.**NOTICE****Unlimited program runtime.**

A time adjustment of 99:59:59 in program step No 10 is equal to an unlimited program runtime.

⇒ If necessary, stop process by pressing **Start/Stop** key.

Create a program

NOTICE**Input only enabled for 5 seconds.**

The time frame for inputs is 5 seconds. If this time expires without any input, the edit frame (= input enabled) returns to bar marking. Only input confirmed by selection knob will be stored.

⇒ First of all write down the complete program. Take these notes in order to carry out programming quickly and uninterrupted.

→ Example
Creating a new
program

Program						1
No	hh:mm:ss	Vac	Vent.	Step	Auto	
01	00:00:00	0				
02	00:00:00	0				
03	00:00:00	0				
04	00:00:00	0				
05	00:00:00	0				
06	00:00:00	0				
07	00:00:00	0				
08	00:00:00	0				
09	00:00:00	0				
10	00:00:00	0				
----- back -----						
00:00:00						

Program						2
No	hh:mm:ss	Vac	Vent.	Step	Auto	
01	00:00:00	0				
02	00:00:00	0				
03	00:00:00	0				
04	00:00:00	0				
05	00:00:00	0				
06	00:00:00	0				
07	00:00:00	0				
08	00:00:00	0				
09	00:00:00	0				
10	00:00:00	0				
----- back -----						
00:00:00						

1. Open program editor → see **7.2.2 Edit program**.
2. Turn the selection knob and place the bar marking onto the line of program step No 01.

Program						3
No	hh:mm:ss	Vac	Vent.	Step	Auto	
01	00:00:00	0				
02	00:00:00	0				
03	00:00:00	0				
04	00:00:00	0				
05	00:00:00	0				
06	00:00:00	0				
07	00:00:00	0				
08	00:00:00	0				
09	00:00:00	0				
10	00:00:00	0				
----- back -----						
00:00:00						

Program						4
No	hh:mm:ss	Vac	Vent.	Step	Auto	
01	00:01:00	0				
02	00:00:00	0				
03	00:00:00	0				
04	00:00:00	0				
05	00:00:00	0				
06	00:00:00	0				
07	00:00:00	0				
08	00:00:00	0				
09	00:00:00	0				
10	00:00:00	0				
----- back -----						
00:01:00						

3. Press the selection knob to start editing program step No 01.
 - ☒ Edit frame enabled.
4. Turn the selection knob to set the desired time, e. g., 1 minute and then press selection knob to confirm input.
 - ☒ Edit frame switches to next position.

→ Example
Create a new
program

Program						5
No	hh:mm:ss	Vac	Vent.	Step	Auto	
01	00:01:00	ATM	<input type="checkbox"/>			
02	00:00:00	0				
03	00:00:00	0				
04	00:00:00	0				
05	00:00:00	0				
06	00:00:00	0				
07	00:00:00	0				
08	00:00:00	0				
09	00:00:00	0				
10	00:00:00	0				
----- back -----						
00:01:00						

Program						
No	hh:mm:ss	Vac	Vent.	Step	Auto	
01	00:01:00	ATM	✓	✓		
02	00:00:00	0				
03	00:00:00	0				
04	00:00:00	0				
05	00:00:00	0				
06	00:00:00	0				
07	00:00:00	0				
08	00:00:00	0				
09	00:00:00	0				
10	00:00:00	0				
----- back -----						
00:01:00						

5. Turn the selection knob to set the required vacuum value, e. g., **ATM** and then press selection knob to confirm input.

- ✓ For **ATM** settings **Vent** and **Step** will be set automatically and setting for **Auto** will be skipped.
- ✓ Bar marking onto program step 02.

Program						6
No	hh:mm:ss	Vac	Vent.	Step	Auto	
01	00:01:00	ATM	✓	✓		
02	00:00:00	0				
03	00:00:00	0				
04	00:00:00	0				
05	00:00:00	0				
06	00:00:00	0				
07	00:00:00	0				
08	00:00:00	0				
09	00:00:00	0				
10	00:00:00	0				
----- back -----						
00:01:00						

Program						7
No	hh:mm:ss	Vac	Vent.	Step	Auto	
01	00:01:00	ATM	✓	✓		
02	00:05:00	0				
03	00:00:00	0				
04	00:00:00	0				
05	00:00:00	0				
06	00:00:00	0				
07	00:00:00	0				
08	00:00:00	0				
09	00:00:00	0				
10	00:00:00	0				
----- back -----						
00:06:00						

6. Press the selection knob to start editing program step No 02.

- ✓ Edit frame enabled.

7. Turn the selection knob, to set the desired time, e. g., 5 minutes and then press selection knob to confirm input.

- ✓ Edit frame switches to next position.

Program						8
No	hh:mm:ss	Vac	Vent.	Step	Auto	
01	00:01:00	ATM	✓	✓		
02	00:05:00	10	<input type="checkbox"/>			
03	00:00:00	0				
04	00:00:00	0				
05	00:00:00	0				
06	00:00:00	0				
07	00:00:00	0				
08	00:00:00	0				
09	00:00:00	0				
10	00:00:00	0				
-----		back	-----			
00:06:00						

Program						9
No	hh:mm:ss	Vac	Vent.	Step	Auto	
01	00:01:00	ATM	✓	✓		
02	00:05:00	10				
03	00:00:00	0				
04	00:00:00	0				
05	00:00:00	0				
06	00:00:00	0				
07	00:00:00	0				
08	00:00:00	0				
09	00:00:00	0				
10	00:00:00	0				
-----		back	-----			
00:06:00						

8. Turn the selection knob to set the required vacuum value, e. g., 10 mbar. Afterwards press selection knob repeatedly until the bar marking is placed onto program step 03.
9. For further input do like described above for program step 01 and 02.

NOTICE

If not stored, edited programs be will be deleted from memory store after switching the controller ON/OFF.

⇒ Save the edited program under a free program number.

Example: display of a program, which is not yet stored.

Program -

Program - : 1


7.2.3 Store program

IMPORTANT!


⇒ Store the edited program under a free program number.

Store program under a program number

→ Example
Store program

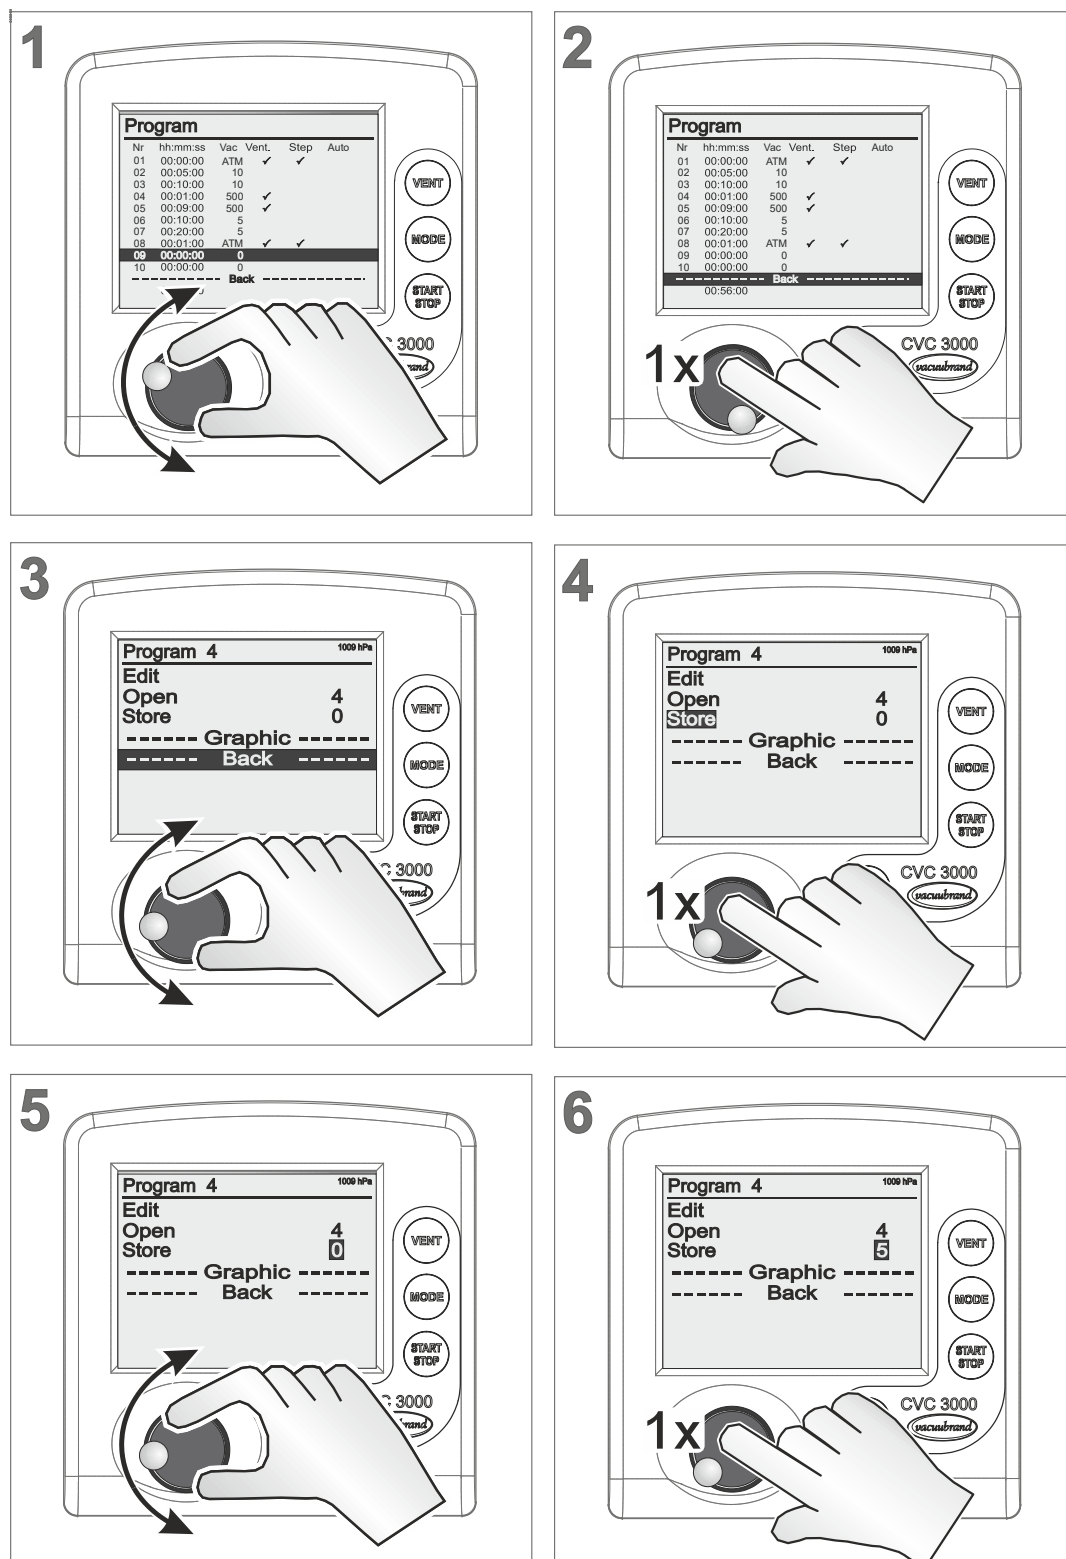

→ Example
Store program

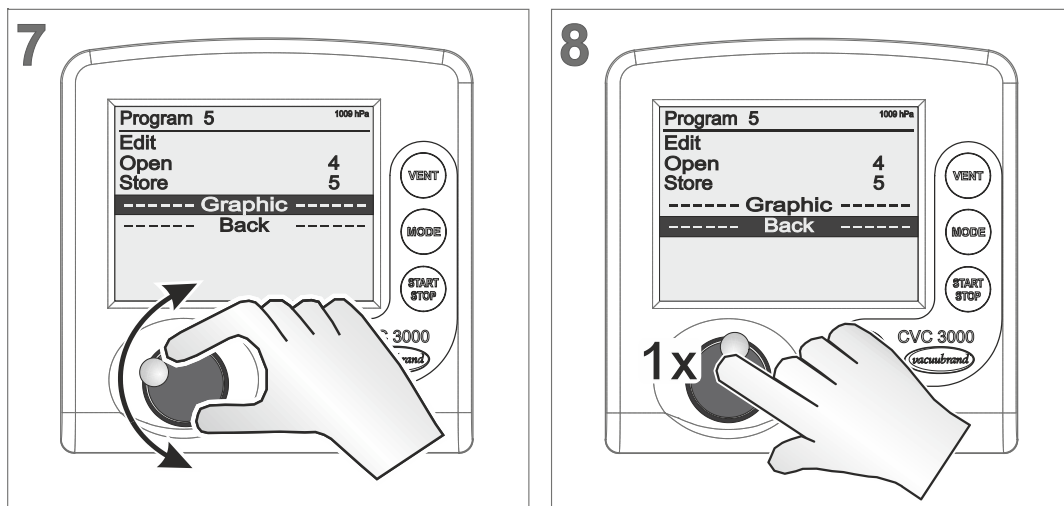

- ✓ Program stored under program number 5.
- ✓ Display switches to pressure display.


7.2.4 Display during operation

Program 1:2

As long as a program is running, the title bar displays additionally the current program step, e. g., Program 1 in program step 02.

Program display during operation

→ Example
Running program
with program steps

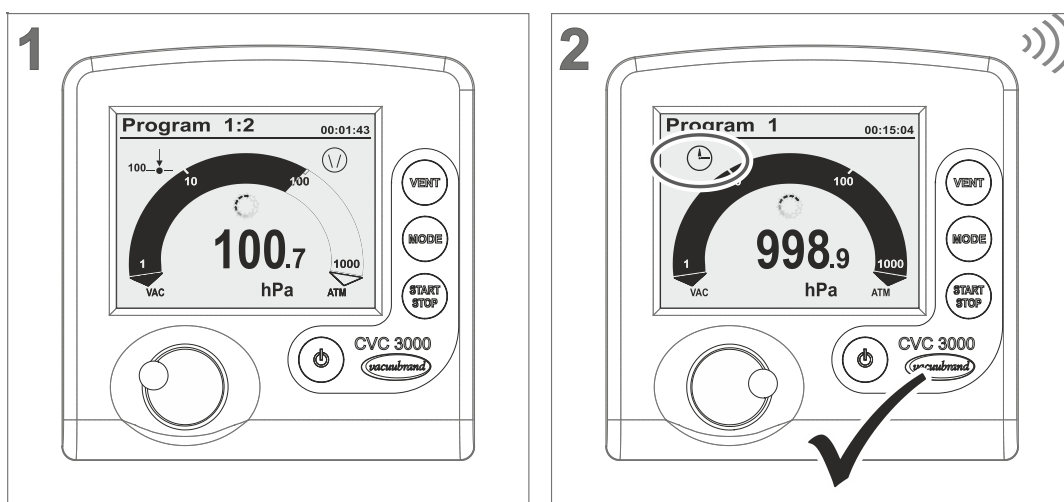

- ✓ Program step blanked.
- ✓ Flashing clock icon = program time elapsed.
- ✓ Warning sound indicates *program time has elapsed*.

⇒ Press **Start/Stop** key, to acknowledge completed program.

7.2.5 Program memory

Meaning The last used process settings remain in the program memory until switching off the controller = temporary buffer.

The program memory provides advantages in practice:

- Operational data in the program memory to repeat the last process in mode **Program**.
- Reproducible test processes: Save the operational data as program directly after process end.
- Facilitate programming, because operational data are already written in the program editor.
- Simple modification of programs for similar processes.

Example: Test procedure for a new substance

→ Example 20 l parallel evaporator and vacuum apparatus:
Test assembly Vacuum controller CVC 3000, in-line suction valve, chemistry diaphragm pump MD 4C NT.

Test procedure In mode **Pump down** the parallel evaporator was quickly evacuated to a vacuum suitable for the substance. At approximately 14 mbar the mode was switched to **Vac control**. The process vacuum for the application was corrected to 10 mbar by quick adaption during operation. Duration of the evaporation was approximately 4.5 hours, afterwards the system was vented to atmosphere pressure.

IMPORTANT!

- ⇒ Save important process data.
- ⇒ Leave the controller switched on after process end and
- ⇒ store successful test values as a controller program.

How to use program memory¹

Test values in temporary buffer

1. Press **Mode** key.
2. Turn selection knob to select **Program**.

☒ Title bar: **Program -**.

3. Open the program editor.

Program					
No	hh:mm:ss	Vac	Vent.	Step	Auto
01	00:00:00	1002	✓	✓	
02	00:05:28	14			
03	00:00:07	10			
04	04:29:11	10			
05	00:00:00	75	✓		
06	00:00:32	75			
07	00:00:00	75			
08	00:00:00	75			
09	00:00:00	75			
10	00:00:00	75			
----- zurück -----					
04:35:08					

☒ Listed values of the latest run test set-up appear.

IMPORTANT!

- ⇒ Set **ATM** as first and last program step. The actual atmospheric pressure may vary. Therefore the setting **ATM** is best suited as initial and final status.
- ⇒ Delete zero times because these program steps will be skipped.

4. Edit data like here in the example:

Modified test values

Program					
No	hh:mm:ss	Vac	Vent.	Step	Auto
01	00:00:00	ATM	✓	✓	
02	00:05:30	14			
03	00:00:07	10			
04	04:30:00	10			
05	00:01:00	ATM	✓		
06	00:00:32	75			
07	00:00:00	75			
08	00:00:00	75			
09	00:00:00	75			
10	00:00:00	75			
----- zurück -----					
04:36:37					

5. Store the program under a free program number.

¹ Not usable for mode VACUULAN.

7.2.6 Program examples

Example 1

Example 1

Program					
No	hh:mm:ss	Vac	Vent.	Step	Auto
01	00:03:00	500			
02	00:00:00	0			
03	00:00:00	0			
04	00:00:00	0			
05	00:00:00	0			
06	00:00:00	0			
07	00:00:00	0			
08	00:00:00	0			
09	00:00:00	0			
10	00:00:00	0			
----- back -----					
00:03:00					

Vacuum pump with in-line isolation valve:

Linear pump down to 500 mbar

N° Program step

- 01 Linear pump down to 500 mbar within 3 minutes. Limited reproducibility because of the undefined initial state.
- 02 -10 not used.

Example 2

Example 2

Program					
No	hh:mm:ss	Vac	Vent.	Step	Auto
01	00:00:00	ATM	✓	✓	
02	00:10:00	300		✓	
03	01:00:00	2			⊥
04	00:01:00	ATM	✓	✓	
05	00:00:00	0			
06	00:00:00	0			
07	00:00:00	0			
08	00:00:00	0			
09	00:00:00	0			
10	00:00:00	0			
----- back -----					
01:11:00					

VARIO® pump with motor speed control connected to rotary evaporator:

Outgassing and automatic distillation with time presettings.

N° Program step

- 01 **ATM** = atmospheric pressure is set as reproducible initial state. The check marks at *Bel.* and *Step* are set automatically when **ATM** is selected.
- 02 Because of the check mark at *Step* the controller pumps down to 300 mbar as quickly as possible and holds vacuum level for 10 minutes at 300 mbar, e. g., solvent degassing.
- 03 The icon at *Auto* effects that the boiling vacuum will be automatically detected within the pressure interval from 300 mbar to 2 mbar. If the process varies, the boiling vacuum will be adapted automatically. The next program step starts after 60 minutes.

- 04 Because of the check mark at *Step* the controller is venting the system as quickly as possible to **ATM**. Control stops after 1 minute.
- 05 -10 not used.

Example 3

Example 3

Program					
No	hh:mm:ss	Vac	Vent.	Step	Auto
01	00:00:00	ATM	✓	✓	
02	00:05:00	10			
03	00:10:00	10			
04	00:01:00	500	✓		
05	00:09:00	500	✓		
06	00:10:00	5			
07	00:20:00	5			
08	00:01:00	ATM	✓	✓	
09	00:00:00	0			
10	00:00:00	0			
----- back -----					
00:56:00					

Vacuum pump with in-line isolation valve and/or Vacuum Management System VMS B:

Pump down with intermediate venting

N° Program step

- 01 **ATM** = atmospheric pressure is set as reproducible initial state.
- 02 Pump down within 5 minutes from **ATM** to 10 mbar (linear ramp).
- 03 Hold vacuum level for 10 minutes at 10 mbar.
- 04 Venting within 1 minute from 10 mbar to 500 mbar.
- 05 Hold vacuum level for 9 minutes at 500 mbar.
- 06 Pump down within 10 minutes from 500 mbar to 5 mbar.
- 07 Hold vacuum level for 20 minutes at 5 mbar.
- 08 Because of the check mark at *Step* the controller is venting the system as quickly as possible to **ATM** = atmospheric pressure. Control stops after 1 minute.
- 09 -10 not used.

7.2.7 Sample form for program

IMPORTANT! When loading the factory settings, the data stored in the program memory will be deleted.

⇒ Keep important program settings and make note of the values that are listed in the program editor.

Program

N°:


No	hh:mm:ss	Vac	Vent.	Step	Auto
01	____:____:____	_____	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
02	____:____:____	_____	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
03	____:____:____	_____	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
04	____:____:____	_____	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
05	____:____:____	_____	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
06	____:____:____	_____	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
07	____:____:____	_____	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
08	____:____:____	_____	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
09	____:____:____	_____	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	____:____:____	_____	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
----- back -----					
	____:____:____				

7.3 Configuration menu

Meaning In menu **Configuration** the controller parameters are set. This menu is also for adjusting the vacuum sensor and for loading **Defaults** settings.

Call up Configuration menu

→ Example
Call up
Configuration menu

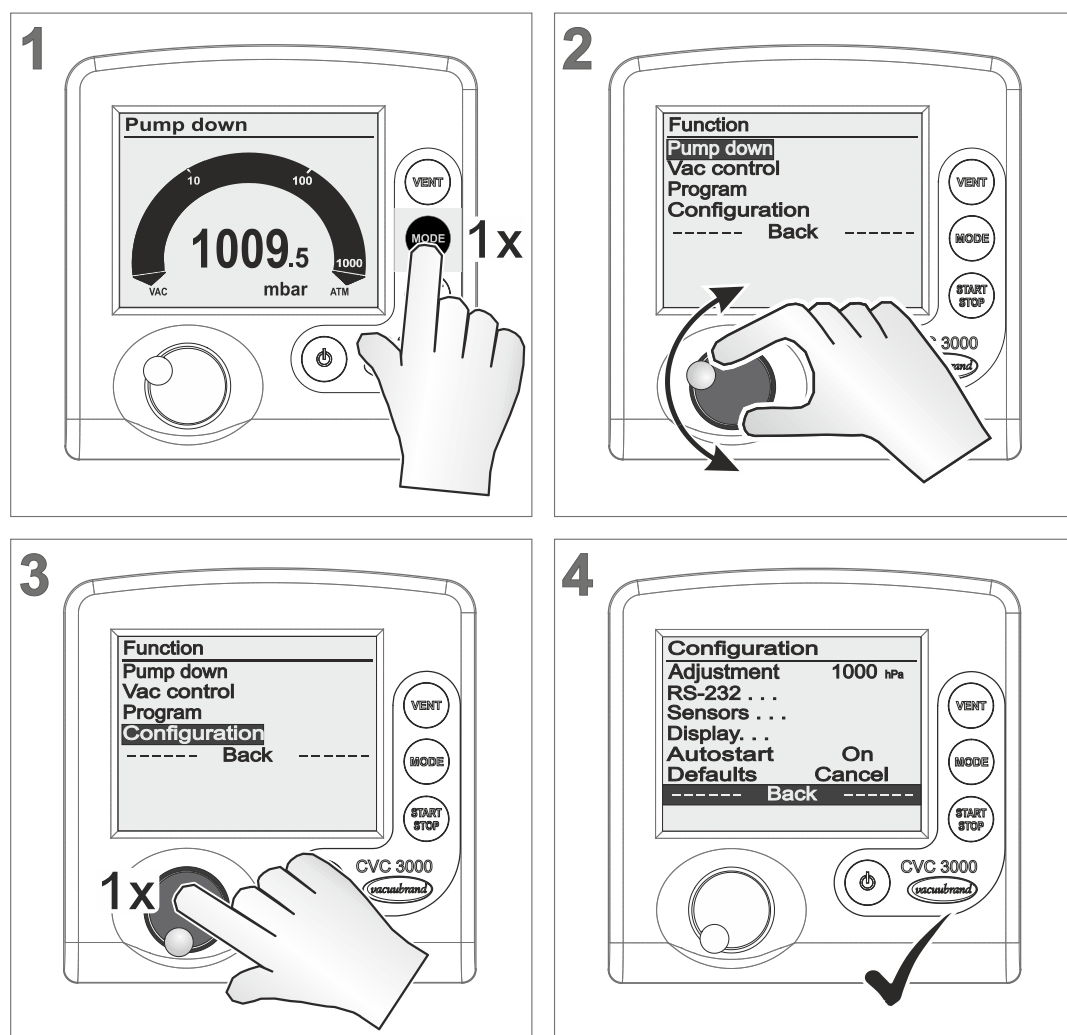

☒ **Configuration** menu displayed.



After 20 seconds without action, the display will return automatically to pressure display.

7.3.1 Content selection

Specified content The following menu items of **Configuration** can be selected, activated and used.

Defaults

Defaults (standard)

Selection	Meaning
Cancel	Leave menu item without default setting.
Load	Load default settings.

IMPORTANT!

If **Defaults Load** is activated all controller parameter will be reset to delivery status. Stored programs will be deleted.

Autostart

Auto start function

Selection	Meaning
Off	After switching on power supply or after power failure the controller remains in <i>Stop</i> . Press Start/Stop key to start the controller.
On	Once power is applied, the controller starts automatically with the settings before power failure. The controller starts control directly without pressing Start/Stop key, if it previously was in running operation. Recommended, if power supply is switched on from a central point or if power is switched on by an external switch.

IMPORTANT!

Ensure, if **Autostart** is activated, that no hazardous situations may occur due to the automatic start of the process.

⇒ Check whether the **Autostart** feature can be used safely with the intended application.

Adjustment

Sensor adjustment
function

Selection	Meaning
1060–700 20–0	Adjustment range of a vacuum sensor, internal or external at atmospheric pressure (1060–700) or under vacuum (20– ~0).

For further descriptions about sensor adjustment

→ see chapter: **9.2 Sensor readjustment**

7.3.2 Submenus

Submenu – Display

Submenu Display

Display		
Brightness	100 %	
Contrast	40 %	
Sound	On	
Units	mbar	
Language	English	
-----	back	-----

Adjustable display
parameter

Parameter	Selection	Meaning
Brightness	0–100 %	Adjust backlight brightness of the display.
Contrast	0–100 %	Adjust display contrast.
Sound	Off	Switch off keystroke sound and warning sound.
	On	Switch on keystroke sound and warning sound.
Units	mbar	Preset pressure unit for user interface.
	Torr	
	hPa	
Language	14 languages available	Select language for user interface.

Submenu – Sensors

In submenu **Sensors** all connected sensors² are listed. The internal sensor is generally displayed as **Sensor**. External sensors are listed with sensor type name and address.

Submenu Sensors

Sensors	
Sensor	990.8 mbar
VSP 1	4.1E+2 mbar

Sensor selection

Display	Meaning
Inverse	Sensor = currently selected for pressure display.
Sensor type	Selection for displaying pressure on basic display (max. 8 sensors are listed).



The display switches automatically to the previous menu when selecting a sensor with the selection knob.

For descriptions about sensor address assignment

→ see chapter: **7.4.2 Submenu Vacuubus (address assignment)**

² -> Reference sensors are not listed in the Sensor menu, but deducted directly from the corresponding VSK sensor.

Submenu – RS-232

Submenu **RS-232** is applied for interface configuration, parameter adjustments and commands.

→ see also chapter: **10.2 Interface commands**.

Submenu RS232

RS-232	
Baud	19200
Parity	8-N-1
Handshake	None
Remote	Off
----- back -----	

Adjustable RS232
parameter


Parameter	Selection	Meaning
Baud	19200	Default setting for transmission speed. The baud rate of data transfer of transmitter and receiver must correspond.
	9600	
	4800	
	2400	
Parity	8-N-1	Default setting for parity check, a method for error detection
	7-O-1	
	7-E-1	
Handshake	RTS-CTS	Preset for continuous data transmission without loss – flow control.
	Xon-Xoff	
	None	
Remote	Off	Control commands not enabled, only queries possible
	On	Connection for communication via RS 232 interface enabled.

IMPORTANT!

When selecting **Remote On** the controller itself is only operable via an external device. All keys of the control panel except key **On/Off** are locked.

VACUU·CONTROL® detects automatically, if **Remote** is activated or deactivated and retains that setting.

Icon on
controller display


Icon	Meaning
	PC icon? Controller in remote operation! Reset Remote: Switch-off Remote (switch off and on controller, press selection knob shortly while booting, select Configuration/RS232/Remote and adjust Off).

7.4 Function menu

Meaning **Function** menu is not for every day use but for special controller parameters, like **VACUU-BUS®** address assignment or updates.

Call up Function menu

→ Example
Call up
Function menu

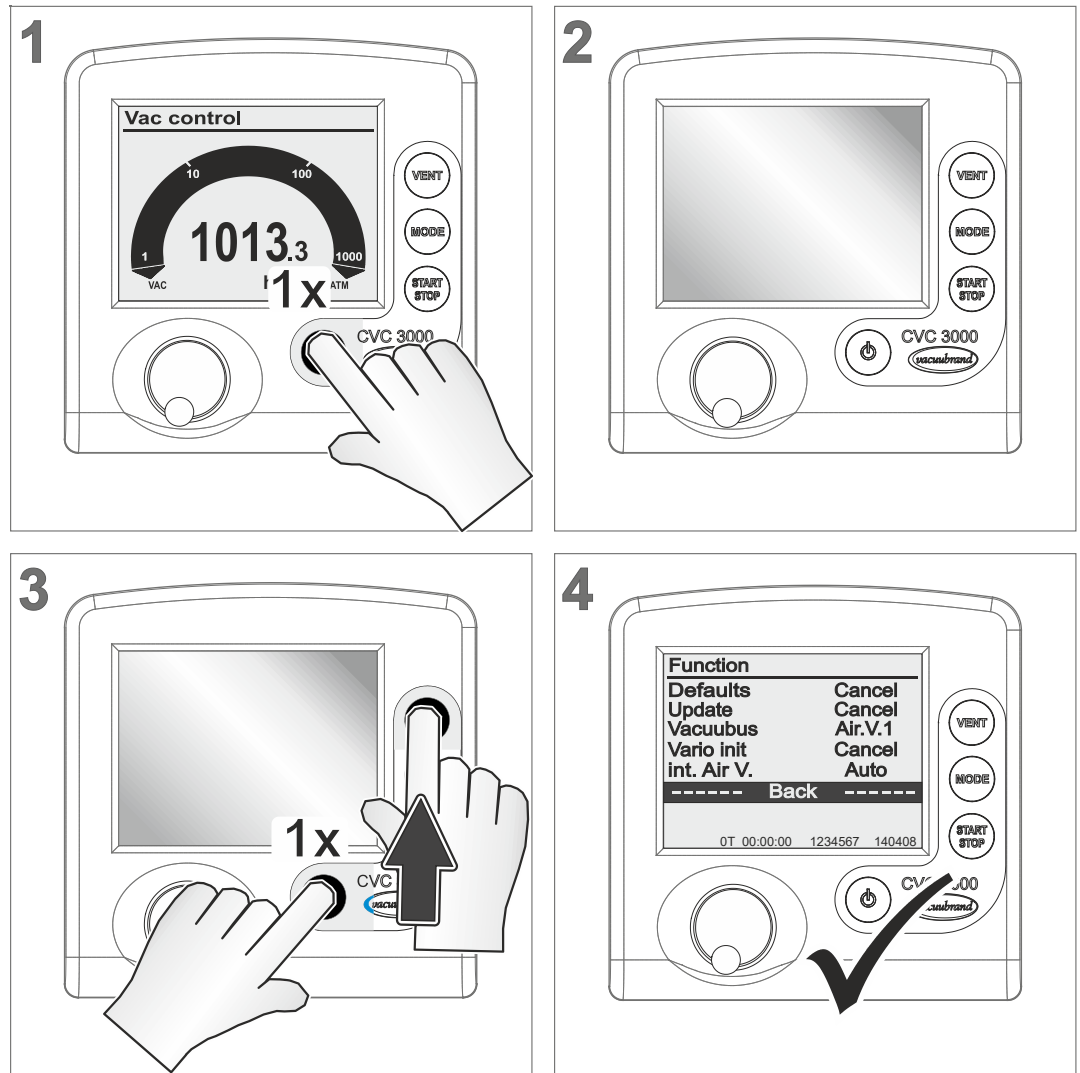

☑ **Function** menu displayed.

7.4.1 Content selection

Specified content The following menu items of **Function** can be selected and/or loaded.

int. Air V.

Internal air
admittance valve
(venting valve)

Selection	Meaning
Auto	Internal venting valve does not switch, if an external venting valve or vacuum sensor is connected to the controller.
Off	Internal venting valve deactivated. Venting function is cannot be controlled. VENT key is switched off.
On	Internal venting valve does switch, even if an external venting valve or vacuum sensor is connected to the controller. VENT key is switched on.

IMPORTANT!

When **Venting** with inert gas ensure that inert gas is connected to all venting valves to prevent intruding air.

Vario init

Initialize frequency
converter

Selection	Meaning
Cancel	Quit menu item without initialization.
NT	Initialization for 2/4 or 8 head NT VARIO diaphragm pump and transferring motor parameter.
Star	Initialization for 8 head VARIO-B diaphragm pump.

IMPORTANT!

Use this function only after the exchange of a frequency converter. Wrong motor parameters may cause motor overheating or bad pumping speed performance.

⇒ Only select motor parameter that is suitable for the vacuum pump.

The set of motor parameters will only be transmitted with the correct key combination.

⇒ Press and hold **Mode** key + press **Selection knob**.

☒ **Succeed** appears on the display.

Update

Firmware update

Selection	Meaning
Cancel	Quit menu item without updating.
Load	Load controller firmware update.

Defaults³

Default settings for
Service

Selection	Meaning
Cancel	Quit menu item without default setting.
Normal	Load default settings – including presettings for 1–3 stage VARIO ® pumps or for pumping units or for table top controller with 2-point control. Presetting: Mode Vac control Set vacuum: 100 mbar
Turbo	Load default settings – including presettings for 4 stage VARIO ® pumps used as backing for turbomolecular pumps. Presetting: Mode Vac control Set vacuum: <i>Turbo</i>
VCL	Load default settings – including presettings for pumping units with built-in controller or for VACUU·LAN with built-in controller. Presetting: Mode VACUULAN Set vacuum: 25 mbar

IMPORTANT!

This type of **Defaults** factory setting resets all controller parameters back to a special pre-configured delivery state.

These factory settings are reserved only for our service technicians.

⇒ Use factory setting in **Configuration** menu.

³ -> Characteristic: When loading **Defaults** in **Function** menu, firstly **Succeed** is displayed, then the language selection appears on the display.

7.4.2 Submenu Vacuubus (address assignment)

NOTICE

VACUU-BUS® components always need to be configured, if several components of the same type are to be connected, e.g., 3 external sensors VSK type. Configuration is equivalent to address assignment.

Address assignment (configuration)


Meaning

Several **VACUU-BUS®** components of the same type, which are connected to the controller, each require an individual address code for correct communication. On delivery state each **VACUU-BUS®** component has the default address 1.

The controller requires the address information to differentiate between identical **VACUU-BUS®** components and for communication. To change address use menu *Function/Vacuubus*.

Example: VACUU-BUS® addresses

→ Example
Assigned address
numbers

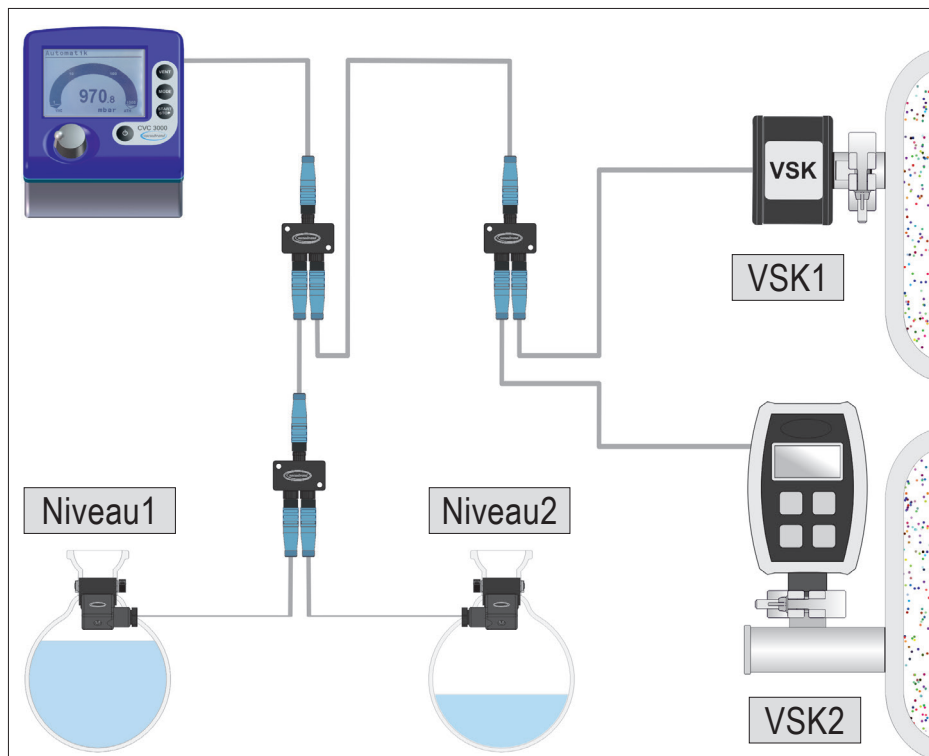

Controller (internal sensor VSK type) + 2x external sensor
+ 2x Level sensor

- New address assignment for the second level sensor and the second external VSK sensor.

Assign a new address number to a VACUU-BUS® component


In the following example a second VSK type sensor receives **VSK2** as new communication address code.

IMPORTANT!







A new address can be assigned **only individually**.

- ⇒ Connect only the **VACUU-BUS®** component to the controller, which requires a new address.
- ⇒ If an address assignment for several **VACUU-BUS®** components of the same type is necessary, then connect and address them individually and one after the other.

→ Example
Assignment for VSK

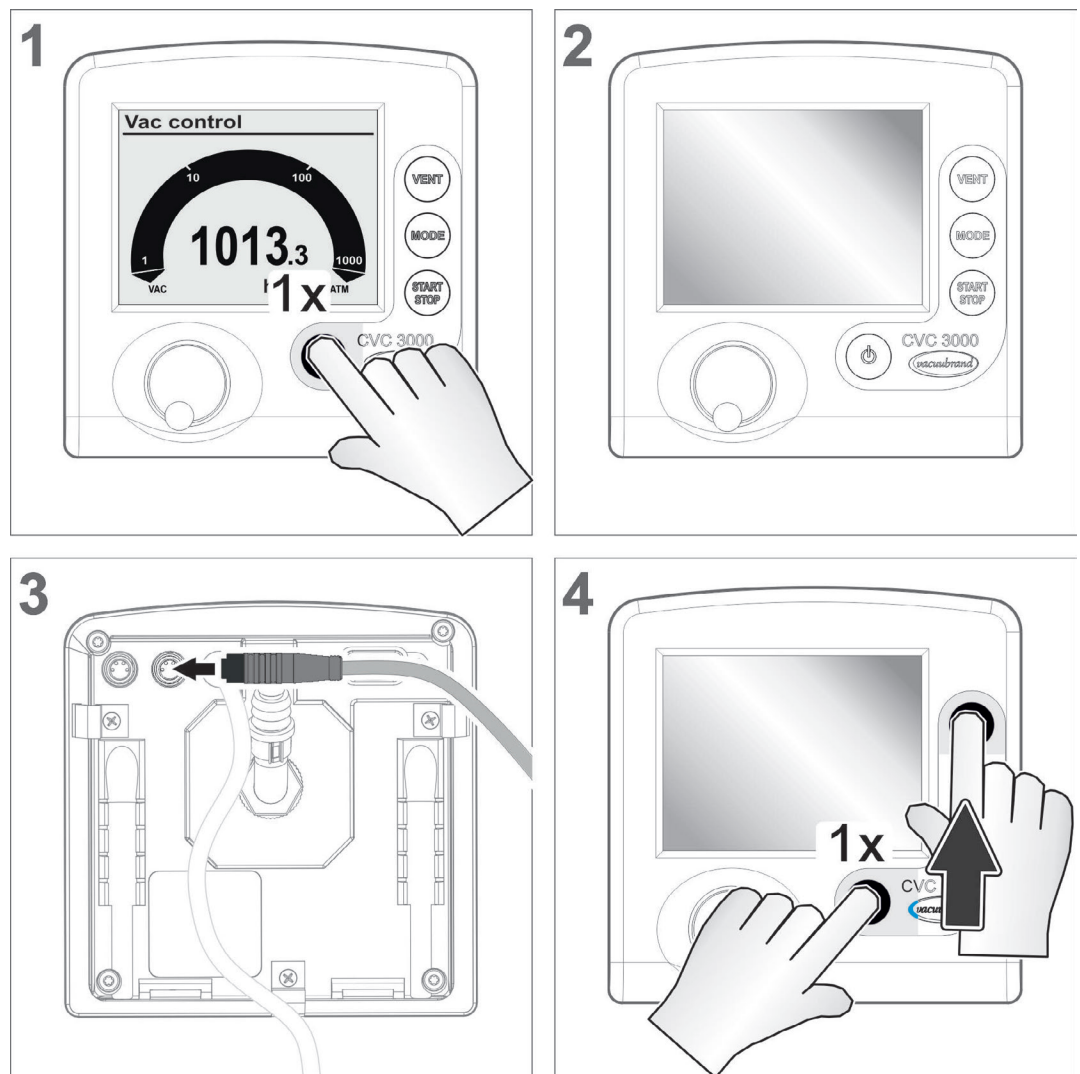

→ Example
VACUU·BUS
assignment

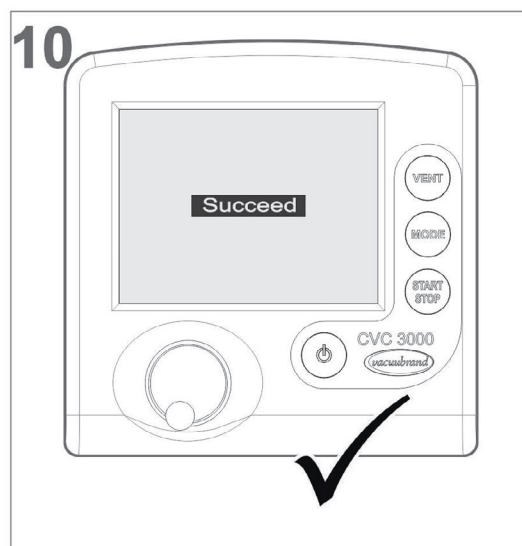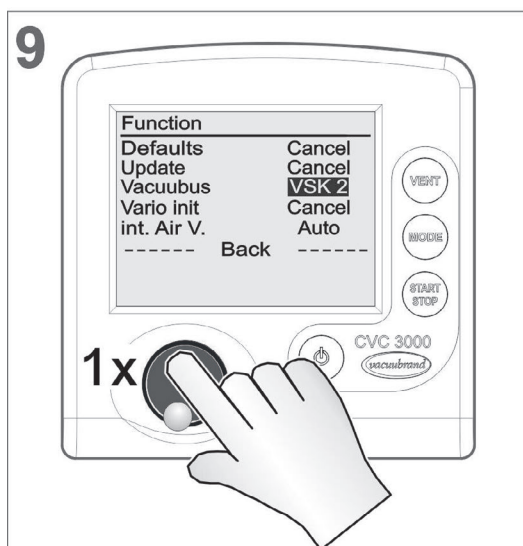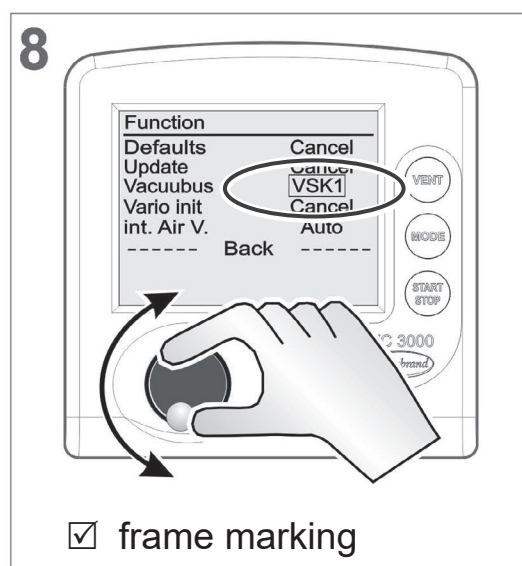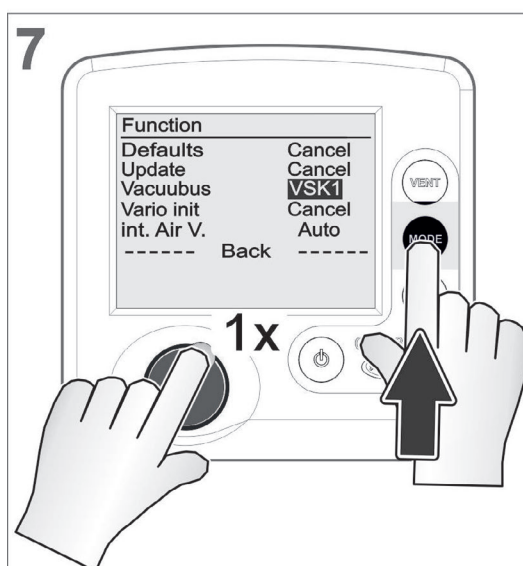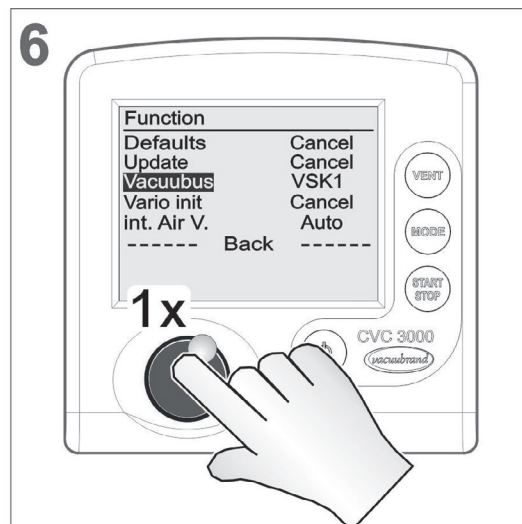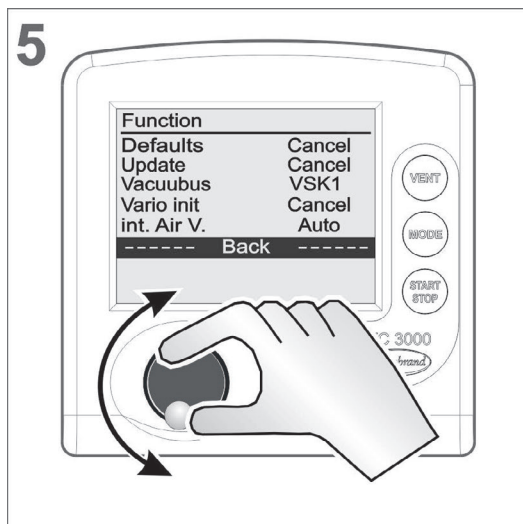

☑ New communication address code for second sensor
VSK = **VSK2**

7.4.3 Possible address configurations

Address table
VACUU·BUS
components

VACUU·BUS elements	**Address N°	Abbreviation
In-line suction valve	1–4	Isol.v. _
Coolant valve	1–4	Waterv. _
Venting valve (air admittance valve)	1–4	Air V. _
VMS module	1–4	VMS _
Fault indicator	1	Error
Remote module	1	Remote
A valve that opens at the end of the process	1–2	End
Not in use	---	Reserved
Level sensor	1–4	Level _
Reference sensor VSK 3000, VACUU·VIEW	1–4	Ref. _
Vacuum sensor VSK 3000, VACUU·VIEW	1–4	VSK _
Vacuum sensor VSP 3000, VACUU·VIEW extended	1–4	VSP _
*Output actual vacuum	1	Vacuum
*Output actual speed	1	Speed
*Input set vacuum and output actual vacuum	1	Set vac
*Input set speed and actual speed	1	SetSpeed
***ATEX-VARIO pump [1500 rpm]	1–3	ATEX _
***Basic configuration Ex; with ATEX VARIO pump [1500 rpm] and Ex sensor	-	ATEX I/O
NT VARIO pump, from 2015 [2400 rpm]	1–4	VarioX _
PC 3001	1–8	Var-SP _
EK Peltronic	1–3	Pelt. _
Not in use	---	Reserved
NT VARIO pump	1–8	Vario _

* Analog I/O module (0–10 V/0–10 V)

** = Number of addresses that can be assigned maximally

*** Analog I/O module (4–20 mA/0–10 V)



The scope of the listed Vacuubus components depends on the firmware version of your controller.

7.5 Differential pressure measurement

Meaning A differential pressure between two pressure sensors can be determined and displayed between the internal pressure sensor and an external sensor⁴ or between two external sensors⁴ → see chapter: *7.4.2 Submenu Vacuubus (address assignment)*. Mode **Vac control** controls automatically to the differential pressure, if the sensor **VSK..** is selected as active sensor in submenu **Sensors...** .

Prepare the internal sensor and one external VSK sensor

- Prepare sensors**
1. Connect an external VSK type sensor to the controller.
 2. Assign the address **Ref.1** for that external sensor.

IMPORTANT!

For differential pressure measurement between the internal sensor and the external sensor, no further sensor with address **VSK1** must be connected.

⇒ Assign other address numbers for additionally connected VSK sensors → see *7.4.2*.

Prepare two external VSK sensors

1. Connect two external sensors VSK type to the controller.
2. Assign address **VSK1** to one of the sensors.
3. Define the second sensor as reference sensor by assigning address **Ref.1** to it.

IMPORTANT!

If address 1 has already been assigned, you should assign the next free address numbers, e. g., **VSK2** and **Ref.2** to the sensors.

The differential pressure is only determined between sensors with corresponding address numbers.

Measuring differential pressure

Measuring differential pressure

- ⇒ Start the controller.
- ☒ Pressure display displays differential pressure: reference sensor *minus* VSK sensor.

⁴ -> VSK 3000 or VACUU·VIEW

8 Resolving problems

Technical support

Technical support

⇒ To identify errors and potential remedies, please refer to the troubleshooting table: ***Fault – Cause – Remedy***.



In case you need additional assistance, please contact our [Service](#) department.

8.1 Error display

The major symbol for fault indication is the warning triangle. Additionally displayed icons and sounds refer to the cause of fault.


Safety alert symbol

Warning triangle

Icon	Meaning
	Flashing: Warning! Where applicable with: <ul style="list-style-type: none"> flashing component icon, warning sound (only when switched on) or flashing backlight.
	<ul style="list-style-type: none"> in combination with number = VACUU·BUS address of the component which is defective.





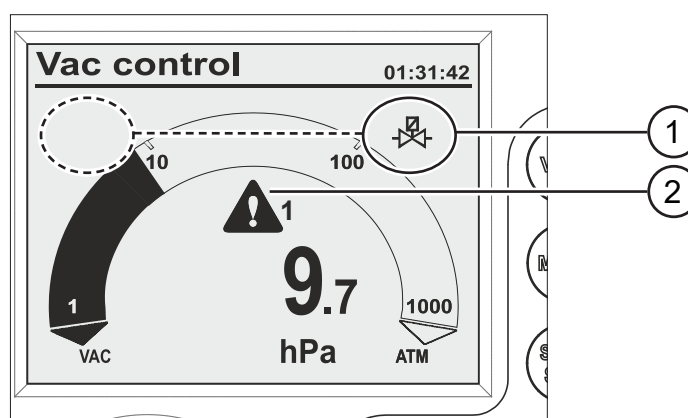





























Example display in case of error

→ Example
Error In-line valve 1



- 1 Possible positions for flashing component/display icon; here: warning In-line valve
- 2 Flashing: Warning triangle

Combinations of flashing display icons

Icon flash rate 	Fault and Meaning	beep when Sound On
	▶ Limit pressure reached	1x 
	▶ Overpressure	1x 
	▶ Process time elapsed	1x 
 + 	▶ Venting valve	2x 
 + 	▶ In-line suction valve	3x 
 + 	▶ Coolant valve	4x 
	▶ External sensor removed ▶ or defective	5x 
	▶ internal sensor defective	7x 
 + 	▶ Vario pump	6x 
 + 	▶ VACUULAN process pressure not reached within 99 hours.	8x 
	Digital I/O module: ▶ Fault indicator triggered or ▶ fault special configurations	9x 
 + 	▶ Level sensor triggered; flask full	10x 
 + 	▶ Emission condenser Peltronic (too hot)	11x 
	 ▶ Analog I/O module	12x 



A defective I/O module, which is configured as a remote module, does not trigger a warning alert. The control is stopped. Alert display by the flashing warning triangle.

8.2 Fault – Cause – Remedy

Fault	Possible cause	✓ Remedy	Personnel
Sensitive process not controllable	<ul style="list-style-type: none"> ▶ Motor speed too high. ▶ Pumping speed too high. 	<ul style="list-style-type: none"> ✓ Reduce motor speed. 	User, Specialist
Frequent error messages of connected components	<ul style="list-style-type: none"> ▶ Several controllers are connected. ▶ Several VACUU·BUS components of the same type are using the same address. 	<ul style="list-style-type: none"> ✓ Use only one controller for one VACUU·BUS system. ✓ Assign individual addresses in menu Function/Vacuubus to components of the same type. 	respon. Specialist
VENT key does not work	<ul style="list-style-type: none"> ▶ Venting function deactivated. 	<ul style="list-style-type: none"> ✓ Check why Venting is deactivated. 	Specialist, respon. Specialist
Internal air admittance valve cannot be triggered	<ul style="list-style-type: none"> ▶ In menu Function, setting of int.Air V is switched Off or Auto. ▶ External air admittance valve is connected, <i>and/or</i> ▶ external vacuum sensor is connected. 	<ul style="list-style-type: none"> ✓ Check if Venting by internal air admittance valve can be used without risk. ✓ Venting safe? Enable the function in menu Function/ int.Air V; adjustment: Auto or On. 	
Internal air admittance valve does not switch	<ul style="list-style-type: none"> ▶ Air admittance valve is soiled. 	<ul style="list-style-type: none"> ✓ Clean air admittance valve, see description in chapter 9.1 Cleaning 	Specialist
Function or menu item cannot be used	<ul style="list-style-type: none"> ▶ Function or menu item possibly only usable with shortcut (key combination). 	<ul style="list-style-type: none"> ✓ Press the correct key combination; for descriptions of keys and shortcuts see chapter: 5.1 Operating elements 	Specialist, respon. Specialist
Vario pump icon flashes	<ul style="list-style-type: none"> ▶ VARIO pump and VMS are both connected at the same time. ▶ VARIO pump defective. ▶ VMS defective or cable is not connected. ▶ Cable break. 	<ul style="list-style-type: none"> ✓ Remove VMS from VARIO-pump and restart controller. ✓ Check VARIO pump for defective parts. ✓ Check VMS for defective parts. ✓ Check cable connections. ✓ Replace defective parts. 	Specialist
Air admittance valve icon flashes	<ul style="list-style-type: none"> ▶ External air admittance valve removed. ▶ Plug disconnected. ▶ External air admittance valve defective. 	<ul style="list-style-type: none"> ✓ Check the connection. ✓ Check plug connection. ✓ Replace defective parts. ✓ Use internal air admittance valve. ✓ Reconfiguration without air admittance valve. 	Specialist

Fault	► Possible cause	✓ Remedy	Personnel
In-line suction valve icon flashes	<ul style="list-style-type: none"> ► In-line suction valve removed. ► Plug disconnected. ► In-line suction valve defective. 	<ul style="list-style-type: none"> ✓ Check the connection. ✓ Check plug connection. ✓ Replace defective parts. ✓ Reconfiguration without In-line suction valve. ✓ Switch-off the controller; On/Off key. ✓ Remove In-line suction valve and ✓ switch on controller again. 	User, Specialist
Coolant valve icon flashes	<ul style="list-style-type: none"> ► Coolant valve removed. ► Coolant valve defective. 	<ul style="list-style-type: none"> ✓ Check the connection. ✓ Replace defective parts. ✓ Reconfiguration without coolant valve. 	Specialist
Level sensor icon flashes	<ul style="list-style-type: none"> ► Level sensor triggered (flask full). ► Level sensor removed. ► Level sensor triggered with empty flask. ► Cable break. ► Level sensor defective. 	<ul style="list-style-type: none"> ✓ Empty flask/catch pot. ✓ Check position of level sensor. ✓ Adjust level sensor or delete the sensor from controller (by loading default). ✓ Check plug connection. ✓ Replace defective parts. 	Specialist
Peltronic icon flashes	<ul style="list-style-type: none"> ► Peltronic emission condenser too hot. ► Plug disconnected. 	<ul style="list-style-type: none"> ✓ Let the Peltronic emission condenser cool down. ✓ Check plug connection. 	User, Specialist
Title bar without text	<ul style="list-style-type: none"> ► No controllable device connected (In-line suction valve, VMS, VARIO pump). 	<ul style="list-style-type: none"> ✓ Check device connections and cable. ✓ Replace defective parts. ✓ Connect a controllable device to the controller. ✓ Use the controller as measuring gauge. 	Specialist
No key reaction – only On/Off, PC icon displayed	<ul style="list-style-type: none"> ► Remote switched On. ► Controller only controllable via connected external end device (via RS232). 	<ul style="list-style-type: none"> ✓ Reset Remote: Switch-off Remote (switch off and on controller, press selection knob shortly while booting, select Configuration/RS232/Remote and adjust Off). ✓ Control controller via end device like PC. 	Specialist
No reaction to key actuation	<ul style="list-style-type: none"> ► Controller defective 	<ul style="list-style-type: none"> ✓ Contact Service and ✓ return device for repair. 	respon. Specialist

Fault	Possible cause	Remedy	Personnel
No display	<ul style="list-style-type: none"> ▶ Controller switched off. ▶ Power supply disconnected. ▶ Power supply not correctly connected. ▶ Mains voltage failure. ▶ Controller defective. ▶ Cable break. 	<ul style="list-style-type: none"> ✓ Switch on the controller; On/Off key. ✓ Check plug connection and wall power supply for correct connection. ✓ Replace defective parts. ✓ Contact Service and ✓ return device for repair. 	Specialist
Blank display	▶ Too many devices connected, e. g., valves.	<ul style="list-style-type: none"> ✓ Power input of all connected devices may not exceed the maximum power consumption of the controller: <ul style="list-style-type: none"> - controller with wall power supply max. 30 W, - controller + VARIO max. 25 W. 	respon. Specialist
	▶ Short circuit of a connected device.	<ul style="list-style-type: none"> ✓ Replace defective parts. 	
	<ul style="list-style-type: none"> ▶ Short circuit at RS232 interface. ▶ Controller defective. 	<ul style="list-style-type: none"> ✓ Check RS232 plug connection. ✓ Contact Service and ✓ return device for repair. 	
Incorrect pressure display	<ul style="list-style-type: none"> ▶ Humidity inside the vacuum sensor. ▶ Vacuum sensor soiled. ▶ Vacuum sensor not adjusted. ▶ Vacuum sensor not correctly adjusted. 	<ul style="list-style-type: none"> ✓ Identify and remove source of humidity. ✓ Dry the vacuum sensor, e. g., by pumping down. ✓ Clean the vacuum sensor, <i>see chapter 9.1 Cleaning</i>. ✓ Readjust vacuum sensor. 	User, Specialist
Digital pressure gauge flashes	<ul style="list-style-type: none"> ▶ Pressure display flashing with 0.0: <ul style="list-style-type: none"> - vacuum adjustment not correctly carried out. ▶ Pressure display flashing: <ul style="list-style-type: none"> - Overpressure! Pressure > 1060 mbar. 	<ul style="list-style-type: none"> ✓ Readjust internal or external vacuum sensor, <i>see chapter 9.2 Sensor readjustment</i>. <p>⚠ WARNING! Risk of bursting. ⇒ Discharge the system immediately by venting.</p>	Specialist
No digital pressure reading	<ul style="list-style-type: none"> ▶ External vacuum sensor defective. ▶ External vacuum sensor removed. ▶ Internal vacuum sensor defective. 	<ul style="list-style-type: none"> ✓ Replace defective parts. ✓ Reconnect external vacuum sensor. ✓ Contact Service and ✓ return device for repair. 	respon. Specialist

Fault	► Possible cause	✓ Remedy	Personnel
Sensors submenu is permanently displayed	► Submenu <i>Sensors...</i> does not automatically switch back to previous display.	✓ Select the required sensor by turning and pressing selection knob.	User, Specialist
After loading defaults <i>Language selection</i> appears	► Special factory settings have been loaded.	✓ Set language and pressure unit. IMPORTANT: Check if the loaded default settings are suitable for your vacuum apparatus. Compare <i>Content selection</i> in chapter: 7.4.1	respon. Specialist
Error I/O module	► Plug disconnected. ► An error occurred in the system, the I/O module passed the error alert to the controller.	✓ Check plug connection. ✓ Remedy external fault.	Specialist, respon. Specialist
VSP sensor displays wrong values	► VSP sensor configured as VSK.	✓ Use menu <i>Function/Vacuum-bus</i> to reconfigure the sensor as VSP.	Specialist, respon. Specialist
Controller in operation, pressure display flashes	► VSK sensors are measuring negative difference pressure.	✓ Select an other vacuum sensor in menu <i>Sensors</i> .	User, Specialist

Action required	► Cause	✓ Remedy
Process time elapsed	► All program steps are completed. ► Program end reached.	✓ Acknowledge indication by pressing <i>Start/Stop</i> key.
Flashing clock icon	► Process time elapsed.	✓ Acknowledge indication by pressing <i>Start/Stop</i> key.
Pump down stops, blinking arrow down icon	► Pressure below preset minimum value.	✓ Acknowledge indication by pressing <i>Start/Stop</i> key. ✓ If possible readjust presetting (min.).
Vac control stops, flashing arrow up icon	► Preset maximum value exceeded.	✓ Acknowledge indication by pressing <i>Start/Stop</i> key. ✓ If possible readjust presetting (max.).
Program -	► Program not yet stored.	✓ Store program under a free program number.

8.3 Controller Reset

Auto reset

Automatic reset

The following error indications will be reset automatically with remedy:

- Overpressure
- Process time elapsed
- Limit pressure reached
- Error air admittance valve
- Error Peltronic

Active reset

Reset after action

Several error indications need to be reset manually. Depending on the fault severity different actions are required.

⇒ Press **Start/Stop** key to reset the following error indications:

- In-line suction valve error
- Coolant valve error
- External vacuum sensor removed
- I/O module activated **Error indication**
- external error indicator has triggered via Digital I/O module; assigned as **Error**.
- Level sensor triggered


⇒ Load **Defaults** (standard factory setting) to reset the following error indications:

- Missing set value presetting or VACUU·BUS plug disconnected via Digital I/O module; assigned as **Remote**.
- Level sensor removed and/or VACUU·BUS plug disconnected.


→ see also chapter: **7.3 Configuration menu** for loading **Defaults**

IMPORTANT!⇒ Note the settings of stored programs, before loading **Default**.**Load *Default* settings**

Load factory settings

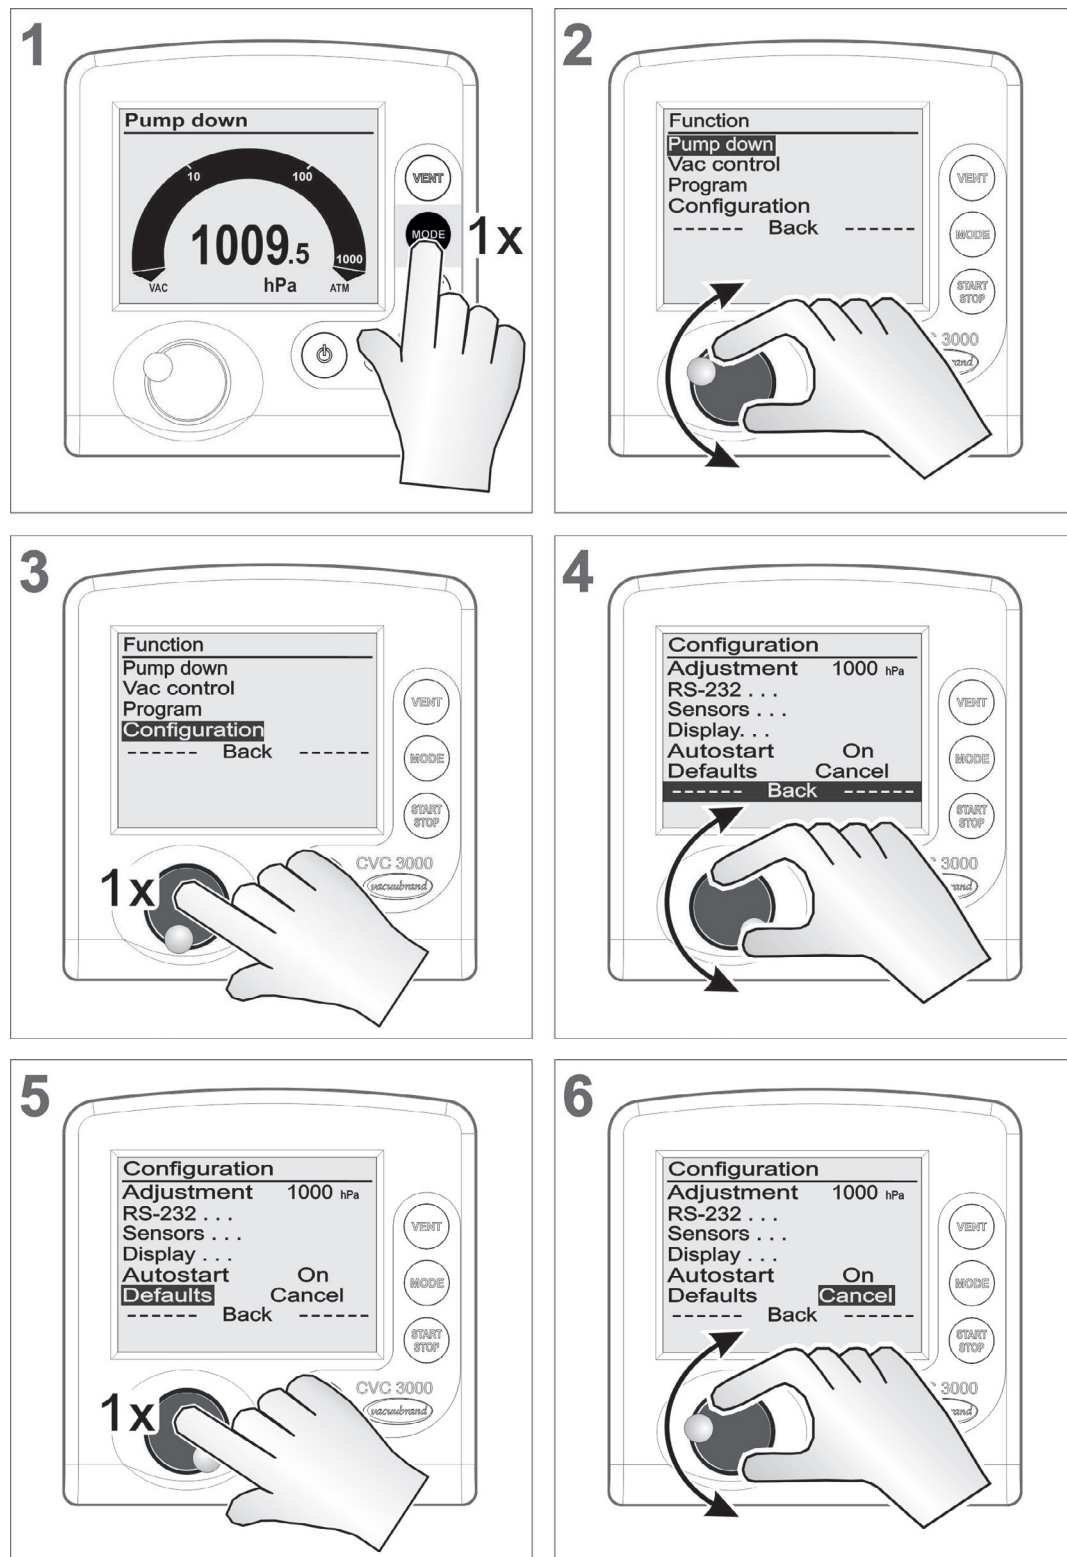

Load factory settings

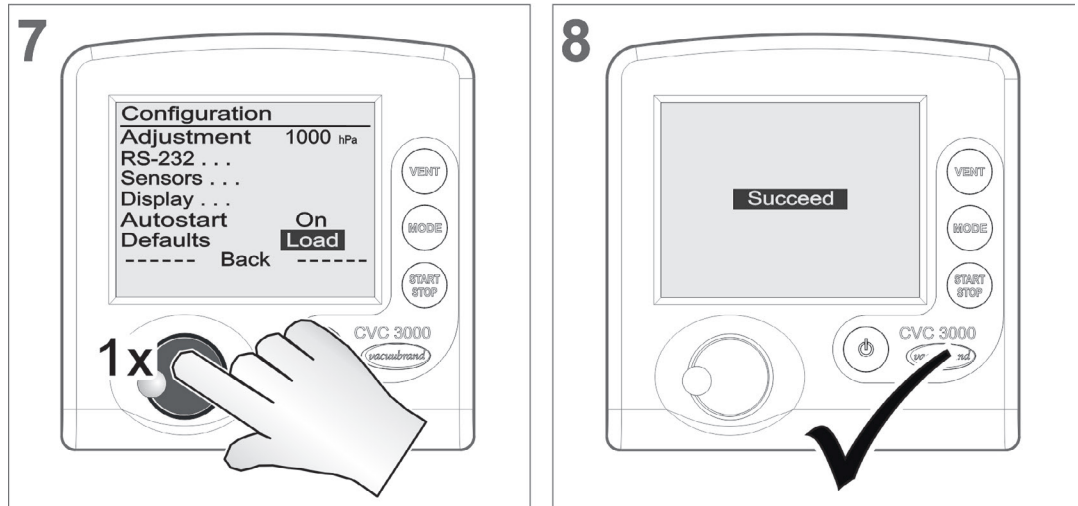

8.4 Error of external components

Error messages for defective external components such as In-line suction valve, vacuum sensor, etc. cannot be reset.

⇒ Replace defective accessories or

⇒ send defective accessories for repair to your local supplier or to our [Service](#).

9 Cleaning and maintenance

9.1 Cleaning

IMPORTANT!

This chapter does not contain descriptions for the decontamination of the controller. This chapter describes only simple cleaning and care measures.

9.1.1 Controller


Clean surface



⇒ Clean soiled surface with a clean, slightly wetted cloth. To moisten the cloth we recommend water or mild soap.

9.1.2 Venting valve

Clean venting¹ valve

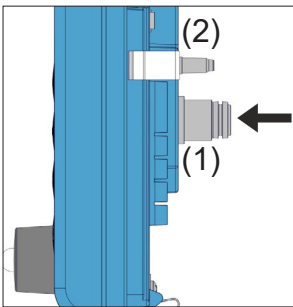

1. Apply slight overpressure of dry air or inert gas to the vacuum port (1).
2. Press the **VENT** key several times until gas escapes through the venting port (2).
3. Repeat this procedure until you hear the clicking of the valve and a gas stream is noticeable at the venting port (2).

9.1.3 Internal sensor

Clean internal sensor

1. Fill a small amount of solvent via the vacuum port (1) in the controller, e. g., cleaning solvent.
2. Let the solvent react for a few minutes.
3. Drain the solvent.
 - ☒ Dissolved substances or discolorations in the solvent are possible.
4. Repeat this procedure until no more pollutants are in the solvent.
5. Let the controller dry.
6. Readjust the internal (vacuum) sensor.

¹ -> air admittance valve

9.2 Sensor readjustment

NOTICE

For readjustment the reference pressures need to be known with certainty

In the pressure range 20 – 700 mbar (15 – 525 Torr) no adjustment is possible.

- ⇒ Check the accuracy of the pressure sensor in case of irregularities in the pressure display.
- ⇒ Readjust the sensor in two steps: at atmospheric pressure and under vacuum.

Do not adjust at atmospheric pressure, if the pressure at the location of the device is not exactly known (pay attention to height above sea level).

Any kind of pollution of the vacuum system, e. g., oil, substances, or humidity could falsify the adjustment.

⇒ Clean polluted sensors before readjustment.

Adjustment at atmospheric pressure

Adjustment at
atmospheric
pressure

An adjustment at atmospheric pressure is only possible if the pressure is higher than > 700 mbar (> 525 Torr).

1. Vent the measurement connection of the controller or in case the connected external vacuum sensor VSK 3000.
2. Make sure that the vacuum sensor (internal or external) is really at atmospheric pressure.
3. Determine the exact atmospheric pressure of your location, e. g., by barometer, inquiry at the meteorological office or the airport.
4. Call up menu **Configuration**.
5. Turn the **selection knob** and place the bar marking on **Adjustment**.
6. Press the **selection knob**.
 - ☒ Marking jumps to numeric value.
7. Adjust the exactly determined local atmospheric pressure by turning the **selection knob**.
8. Press the **selection knob**.
 - ☒ Sensor adjusted to atmospheric pressure.

Adjustment under vacuum

Adjustment under vacuum

An adjustment under vacuum is only possible if the pressure is lower than < 20 mbar (< 15 Torr) absolute.

1. Evacuate the measurement connection of the controller or in case the connected external vacuum sensor VSK 3000 to a pressure $< 0,1$ mbar.

IMPORTANT!

Adjustment under vacuum with an actual pressure higher than $0,1$ mbar (0.1 Torr) reduces the accuracy of the measurement. If the pressure is significantly higher than $> 0,1$ mbar (> 0.1 Torr) the adjustment to a reference pressure is recommended.

2. Call up menu **Configuration**.
3. Turn the **selection knob** and place the bar marking on **Adjustment**.
4. Press the **selection knob**.
 - ☒ Marking jumps to numeric value.
5. Adjust the pressure value to 0 by turning the **selection knob**.
6. Press the **selection knob**.
 - ☒ Sensor adjusted under vacuum.

NOTICE

The readjustment of a VSP 3000 can only be carried out in warmed-up state.

Adjustment is not possible during the warm-up time.

- ⇒ Use a high vacuum pump for the adjustment of a VSP sensor.
- ⇒ After connection to power supply and after the pressure has reached $< 10^{-3}$ mbar, wait 20 minutes before adjusting the VSP sensor.
- ⇒ Carry out the adjustment in the same order as described above for VSK.

Adjustment at a reference pressure

Adjustment at
reference pressure

Instead of adjustment under vacuum to a pressure $< 0,1$ mbar (< 0.1 Torr), adjustment to a precisely known reference pressure within the range of 0 – 20 mbar (0 – 15 Torr) is possible.

1. Evacuate the measurement connection of the controller or in case the connected external vacuum sensor VSK 3000 to a pressure in the range of 0 – 20 mbar (0 – 15 Torr).
2. Call up menu **Configuration**.
3. Turn the **selection knob** and place the bar marking on **Adjustment**.
4. Press the **selection knob**.
 - ☒ Marking jumps to numeric value.
5. Adjust the pressure value to the actual reference pressure by turning the **selection knob**.
6. Press the **selection knob**.
 - ☒ Sensor adjusted to reference pressure.

IMPORTANT!

The measurement uncertainty of the reference pressure will directly affect the measurement uncertainty of the controller.

If the nominal ultimate vacuum of a diaphragm pump is used as reference vacuum, the accuracy of the controller might be doubtful. The diaphragm pump may not achieve the specified vacuum (due to condensate, poor condition, failure of valves or diaphragm, leaks).

For further descriptions about **Adjustment**
→ see chapter: **7.3 Configuration menu**

10 Appendix

10.1 Technical information

Technical
information

Product	
Vacuum controller	Vacuum Controller CVC 3000
Internal vacuum sensor	Ceramic diaphragm (alumina), capacitive, gas independent, absolute pressure

10.1.1 Technical data

Technical data

Ambient conditions		(US)
Working temperature	10–40 °C	50–104°F
Transport- and storage temperature	-10–60 °C	14–140°F
Altitude, max.	3000 m above sea level	9840 ft above sea level
Relative humidity	30–85 %, non condensing	
Degree of protection IEC 60529 (controller front)	IP 20 (IP 42)	
Degree of protection UL 50E		type 1
Avoid condensation or contamination by dust, liquids, or corrosive gases.		

Plug-in power supply	30 W	25 W
Input voltage	100–240 VAC	100–240 VAC
Frequency	50–60 Hz	50–60 Hz
Power consumption, max.	0,8 A	0,7 A
Output current, max.	1,25 A	1,05 A
Output voltage, short circuit proof	24 VDC	24 VDC
Weight	0.3 kg	0.14 kg
Dimensions L x B x H	108 mm x 58 mm x 34 mm 4.3 in. x 2.3 in. x 1.4 in.	71 mm x 57 mm x 33 mm 2.8 in. x 2.2 in. x 1.3 in.
Cable length, approx.	2 m (79 in.)	
Power plug	AC, replaceable: CEE/UK/US/AUS	

Electrical data – CVC 3000		(US)
Supply voltage, max.	24 VDC (±10 %)	24 VDC (±10 %)
Power, max.	3,4 W	3.4 W
max. admissible current total for connected valves	4 A	4 A

Technical data
basic device

Port (interface)	RS 232 SUB-D 9 poles
Remote control, optional	VACUU·CONTROL®

Vacuum data

CVC 3000, internal vacuum sensor (US)

ATEX approval if the ATEX marking is shown on the rating plate
 II 3/- G Ex h IIC T3 Gc X
 Internal Atm. only
 Tech.File: VAC-EX02
 Inner part (pumped gases)

Measuring range, absolute	1080–0,1 mbar	810–0.1 Torr
max. control range	1060–0,1 mbar	795–0.1 Torr
Resolution	0,1 mbar	0.1 Torr

max. admissible media temperature (gas):

Temporarily	80 °C	176°F
Continuous operation	40 °C	104°F
Measurement uncertainty	< ±1 mbar	< ±0.75 Torr
Temperature coefficient	< ±0,07 mbar/K	< ±0.05 Torr/K

External vacuum sensor VSK 3000

max. admissible pressure, absolute	1,5 bar	1125 Torr
------------------------------------	---------	-----------

Venting

max. admissible pressure, absolute	1,2 bar	900 Torr
------------------------------------	---------	----------

Gas connections

CVC built-in version	Fitting for PTFE tube 10/8 mm
CVC table top version	Fitting for PTFE tube 10/8 mm or hose nozzle for flexible tube DN 6/10
Venting	Hose nozzle for flexible tube $d_i = 4–5$ mm

Technical data
package for fine
vacuum control

Vacuum data (only differing data)

CVC 3000 with external VSP 3000 (US)

Measuring range, absolute	1000–1x 10 ⁻³ mbar	750–1x 10 ⁻³ Torr
max. control range	1000–1x 10 ⁻³ mbar	750–1x 10 ⁻³ Torr

External vacuum sensor VSP 3000

max. admissible pressure, absolute	1,5 bar	1125 Torr
Cable, length	2 m	7 ft

Technical data

Venting		
max. admissible pressure, absolute	1,2 bar	900 Torr
without internal venting valve		
Display		
Type	LC display (LCD)	
Brightness control	yes	
Pressure display	switchable: mbar, Torr, hPa	
Weight and dimensions*		(US)
Weight (built-in)	440 g	0.97 lb
Weight with foot (table top)	570 g	1.3 lb
Dimensions	123 mm x 124 mm x 83 mm 5 in. x 5 in. x 3.5 in.	
Dimensions with foot	144 mm x 124 mm x 115 mm 6 in. x 5 in. x 4.5 in.	

* without wall power supply

10.1.2 Product comparison CVC 3000

Product comparison CVC 3000

Product name	Vacuum controller	internal venting valve	external venting valve	internal vacuum sensor	external vacuum sensor	lower measuring limit (mbar)	Measuring principle - capacitive	Measuring principle - Pirani	Measuring principle - cold cathode	Measuring principle gas type independent	ATEX category 2	ATEX category 3 internal Atm. only
CVC 3000	✓	✓	x	✓	x	0.1	✓	-	-	✓	-	✓
CVC 3000 detect	✓	✓	x	✓	x	0.1	✓	-	-	✓	-	✓
CVC 3000 + VSK 3000	✓	✓	x	-	✓	0.1	✓	-	-	✓	-	✓
CVC 3000 + VSP 3000	✓	-	x	-	✓	1x 10 ⁻³	-	✓	-	-	-	-

x = optionally


10.1.3 Rating plate



- ⇒ In case of malfunction, please note type and serial number on the rating plate.
- ⇒ When contacting our [Service](#) department, name us product type and serial number. With this information we can offer selective support and advice for your product.

Rating plate CVC 3000

Rating plate

Manufacturer	VACUUBRAND GMBH + CO KG
Type/Date of construction/Month	CVC 3000 20 /
Serial number	SN
Power supply	V
Electrical power	W
Compatible to VACUU-BUS	VACUU-BUS
ATEX spec *	Ex Tech File: Internal Atm. only
Address	 Alfred—Zippe—Str. 4 97877 Wertheim Made in Germany

* Group and category, marking G (gas), type protection, explosion group, temperature class (additionally see: [Approval for ATEX equipment](#)).

10.1.4 Wetted parts

Wetted parts

Component	Wetted materials
Vacuum connection, hose nozzle	PP
Sensor	Aluminium oxide ceramic
Sensor housing	PPS/Glass fiber
Sensor seal	chemically resistant fluoroelastomer
Venting valve seal	FFKM

10.2 Interface commands

Short description
interface commands

The command set is based on NAMUR recommendations. In the delivery state it is fully compatible with the previous controller CVC 2000. Operation programs for CVC 2000 are able to communicate with CVC 3000 (pay attention to interface settings).

→ see also: **Submenu – RS-232**

The advanced command set of CVC 3000 can be used for full functionality (switch by CVC 3<CR>). CVC 3000 commands which are not listed for CVC 2000 also work for CVC 2000 command set (e. g., IN_SP_).

All commands are written in capital letters with angle brackets: <CR>, <CR><LF> or <LF>. Value entries are separated from command by blank and may be shortened to relevant digits (e. g., 5, 05, 005, 0005 identical for pressure presets).

The output of the controller is always with complete number of digits and leading zeros.


Set point commands are only allowed in remote mode. Whether a command has been executed correctly can be checked by IN_STAT. Via ECHO command an auto-reply of the transmitted parameter can be switched on. The set point commands REMOTE and CVC 2/3 are always possible.

For safe operation send maximum 10 commands per second.

10.2.1 Pin assignment (RS232)

Sub-D panel connector

SUB-D 9 poles

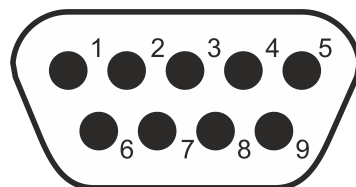

Sub-D 9 poles
(rear side of CVC 3000)

PIN	Name	Operation	PIN	Name	Operation
1	DCD	---	6	DSR	---
2	RxD	Received data	7	RTS	Transmission request
3	TxD	Transmission data	8	CTS	Ready to send
4	DTR	+10 V	9	RI	+5 V (Bluetooth, remote control)
5	GND	Mass	-	---	---

10.2.2 Read commands (CVC 2000)

Command	Operation	Reply	Description
IN_PV_1	actual pressure	XXXX mbar/hPa/Torr	unit corresponding to default settings
IN_PV_2	motor speed	XX.X Hz	actual motor speed
IN_CFG	default settings	0XXXX	VACUU·LAN
		1XXXX	continuous pumping
		2XXXX	controlling without auto mode
		3XXXX	controlling by auto mode
		4XXXX	program
		X0XXX	no coolant valve
		X1XXX	coolant valve
		XX0XX	no air admittance valve
		XX1XX	air admittance valve
		XXX0X	no automatic switch-off
		XXX1X	automatic switch-off
		XXXX0	operation by remote off
		XXXX1	operation by remote on
IN_ERR	error status	1XXX	pump electronics error
		X1XX	overpressure
		XX1X	error at vacuum sensor
		XXX1	last command at interface incorrect
IN_STAT	state of process control	0XXX	coolant valve not triggered (closed)
		1XXX	coolant valve triggered (open)
		X0XX	air admittance valve not triggered (closed)
		X1XX	air admittance valve triggered (open)
		XX00	VACUU·LAN: inactive
		XX01	VACUU·LAN: pump down; set value > default value
		XX02	VACUU·LAN: pump down, timer running
		XX03	VACUU·LAN: stop carried out
		XX10	continuous pumping: inactive
		XX11	continuous pumping: active
		XX20	vacuum control: inactive
		XX21	vacuum control: actual pressure > set pressure
		XX22	vacuum control: actual pressure > set pressure (±1 mbar)
		XX23	vacuum control: actual pressure < set pressure
		XX30	auto mode: inaktiv
		XX31	auto mode: detect boiling point
IN_STAT	state of process control	XX32	auto mode: tracking boiling point
		XX33	auto mode: automatic switch-off carried out
		XX4X	program
		XX5X	gauge mode

10.2.3 Write commands (CVC 2000)

Command	Operation	Parameter	Description
OUT_MODE	operation mode	1	continuous pumping
		2	controls without auto mode
		3	controls by auto mode
		30	<i>optional: sensitivity: low</i>
		31	<i>optional: sensitivity: normal</i>
		32	<i>optional: sensitivity: high</i>
		4	program
OUT_SP_1	set vacuum	XXXX	unit corresponding to default settings (mbar/hPa/Torr); see respective operation for parameter range
OUT_SP_V	set vacuum plus venting*	XXXX	unit corresponding to default settings (mbar/hPa/Torr); see respective operation for parameter range
<i>* Pressure setting with venting is only possible in mode Vac control, if an air admittance valve is connected and configured, and vacuum control is started. The air admittance valve opens automatically if the actual pressure is at least 10 mbar (7.5 Torr) below the preset pressure. Venting function stops, when control is stopped by pressing START/STOP, or when mode is changed. The command OUT_SP_V must be executed anew, if necessary.</i>			
OUT_SP_2	motor speed	XX.X	motor speed in Hz (99.9 for <i>HI</i>)
OUT_SP_3	start-up pressure	XXXX	unit corresponding to default settings (mbar/hPa/Torr); see respective operation for parameter range
OUT_SP_4	delay time	XX:XX	hh:mm (hours:minutes)
OUT_SP_5	switch-off pressure	XXXX	unit corresponding to default settings (mbar/hPa/Torr); see respective operation for parameter range
OUT_SP_6	turn-off time	XX:XX	hh:mm (hours:minutes)
START	start process control	---	---
STOP	stop process control	1	stop process control
		2	stop process control and storing the actual pressure as default value
REMOTE	remote operation**	0	remote off
		1	remote on
<i>** For operation by remote (remote on/off), the user must ensure that no hazardous situation can arise in the system. Especially when due to activated remote direct process control is impossible.</i>			
OUT_VENT	trigger air admittance valve	0	close air admittance valve (not automatically)
		1	open air admittance valve

10.2.4 Read commands (CVC 3000)

Command	Operation	Reply	Description
IN_PV_1	actual pressure	XXXX.X (X.XEXX for Pirani) mbar/hPa/Torr	unit corresponding to default settings; with decimal place for VSK or exponen- tially for Pirani
IN_PV_Sx	actual pressure vacuum sensor x	XXXX.X (X.XEXX for Pirani) mbar/hPa/Torr	pressure of sensor x, unit corresponding to default settings; with decimal place for VSK or exponen- tially for Pirani (sequence of numeration like in display Sensors)
IN_PV_2	motor speed	XXX%	actual motor speed; 1-100% or HI
IN_PV_3	time	XX:XX h:m	process runtime (Stunden:Minuten)
IN_PV_X	pressure	XXXX.X XXXX.X ...	pressure of all connected sensors, unit corre- sponding to default settings (mbar/hPa/Torr)
IN_PV_T	controller uptime	XXXXdXXh	uptime in days and hours
IN_CFG	pre-settings	0XXXXXXXXXXXXXXXXX	VACUU·LAN
		1XXXXXXXXXXXXXXXXX	pump down
		2XXXXXXXXXXXXXXXXX	vac control
		3XXXXXXXXXXXXXXXXX	auto mode
		4XXXXXXXXXXXXXXXXX	program
		5XXXXXXXXXXXXXXXXX	gauge
		XyXXXXXXXXXXXXXXXX	y: 0.....D: language* (hexadecimal)
* language: 0: German, 1: Englisch, 2: French, 3: Italian, 4: Spanish, 5: Turkish, 6: Korean, 7: Chinese, 8: Portugese, 9: Russian, A: Polish, B: Dutch, C: Japanese, D: Finnish			
IN_CFG	pre-settings	XX0XXXXXXXXXXXXXXXX	unit mbar
		XX1XXXXXXXXXXXXXXXX	unit Torr
		XX2XXXXXXXXXXXXXXXX	unit hPa
		XXX0XXXXXXXXXXXXXXXX	auto start off
		XXX1XXXXXXXXXXXXXXXX	auto start on
		XXXX0XXXXXXXXXXXXXXXX	acoustic signal off
		XXXX1XXXXXXXXXXXXXXXX	acoustic signal on
		XXXXX0XXXXXXXXXXXXX	VARIO pump not connected
		XXXXX1XXXXXXXXXXXXX	VARIO pump connected
		XXXXXX0XXXXXXXXXXXXX	VMS not connected
		XXXXXX1XXXXXXXXXXXXX	VMS connected
		XXXXXXX0XXXXXXXXXXXXX	in-line valve not connected
		XXXXXXX1XXXXXXXXXXXXX	in-line valve connected
		XXXXXXX0XXXXXXXXXXXXX	coolant valve not connected
		XXXXXXX1XXXXXXXXXXXXX	coolant valve connected

Command	Operation	Reply	Description
IN_CFG	pre-settings	XXXXXXXX1XXXXXX	coolant valve connected
		XXXXXXXXX0XXXXXX	air admittance valve not connected
		XXXXXXXXX1XXXXXX	air admittance valve connected
		XXXXXXXXX0XXXXXX	fault indicator not connected
		XXXXXXXXX1XXXXXX	fault indicator connected
		XXXXXXXXX0XXXXXX	level sensor not connected
		XXXXXXXXX1XXXXXX	level sensor connected
		XXXXXXXXX0XXXXXX	remote module not connected
		XXXXXXXXX1XXXXXX	remote module connected
		XXXXXXXXXXXXXyXX	y: 1.....9: sensor number (active sensor)
		XXXXXXXXXXXXXyX	y: 1.....9: sensor quantity
		XXXXXXXXXXXXX0	no operation by remote
		XXXXXXXXXXXXX1	operation by remote
IN_STAT	process control status	0XXXXXX	pump off
		1XXXXXX	pump on
		X0XXXXX	in-line valve closed
		X1XXXXX	in-line valve open
		XX0XXX	coolant valve closed
		XX1XXX	coolant valve open
		XXX0XX	air admittance valve closed
		XXX1XX	air admittance valve open
		XXXX0X	VACUU·LAN
		XXXX1X	pump down
		XXXX2X	vac control
		XXXX3X	auto mode
		XXXX4X	program
		XXXX5X	gauge
		XXXXX0	control off
		XXXXX1	pump down - find boiling point
		XXXXX2	set vacuum reached - boiling point found
		XXXXX3	below set vacuum - automatic switch-off
IN_ERR	error status	0XXXXXXXX	no pump error
		1XXXXXXXX	pump error
		X0XXXXXXXX	no in-line valve error
		X1XXXXXXXX	in-line valve error
		XX0XXXXXXXX	no coolant valve error
		XX1XXXXXXXX	coolant valve error
		XXX0XXXXXX	no air admittance valve error
		XXX1XXXXXX	air admittance valve error
		XXXX0XXXXX	no overpressure

Command	Operation	Reply	Description
IN_ERR	error status	XXXX1XXXX	overpressure
		XXXXXX0XXX	no level sensor error
		XXXXXX1XXX	level sensor error
		XXXXXX0XX	no external error
		XXXXXX1XX	external error
		XXXXXXX0X	catch pot not full
		XXXXXXX1X	catch pot full
		XXXXXXXXX0	last interface command correct
		XXXXXXXXX1	last interface command incorrect
IN_SP_1	set vacuum	XXXX mbar/hPa/Torr	unit corresponding to default settings
IN_SP_2	maximum motor speed	XXX%	motor speed in % (1-100% or <i>HI</i>)
IN_SP_3	start-up pressure	XXXX mbar/hPa/Torr	unit corresponding to default settings, start-up pressure for VACUU·LAN or two-point control
IN_SP_4	delay time	XX:XX h:m	hours:minutes (00:00 = off)
IN_SP_5	switch-off pressure	XXXX mbar/hPa/Torr	maximum for vac control, minimum for pump down unit corresponding to default settings
IN_SP_6	runtime	XX:XX h:m	hours:minutes; preset process time
IN_SP_P1y	time	XX:XX:XX h:m:s	hours:minutes:seconds time in program step y (0.....9)
IN_SP_P2y	pressure	XXXX mbar/hPa/Torr	pressure in program step y (0.....9) unit corresponding to default settings
IN_SP_P3y	air admittance valve	0	no air admittance valve in program step y (0.....9)
		1	air admittance valve in program step y (0.....9)
IN_SP_P4y	step	0	no step in program step y (0.....9)
		1	step in program step y (0.....9)
IN_SP_P5y	auto	0	no auto in program step y (0.....9)
		1	auto in program step y (0.....9)
IN_VER	version	CVC 3000 VX.XX	software version

10.2.5 Write commands (CVC 3000)

Command	Operation	Parameter	Description
OUT_MODE	operation mode	0	VACUU·LAN
		1	continuous pumping
		2	vac control
		3	auto mode
		30	<i>optional: sensitivity: low</i>
		31	<i>optional: sensitivity: normal</i>
		32	<i>optional: sensitivity: high</i>
		4	program
OUT_CFG	restart searching Vacuubus device	yXXX	y: 0.....D: language+ (hexadecimal), see: read command CVC 3000: IN_CFG
		X0XX	unit mbar
		X1XX	unit Torr
		X2XX	unit hPa
		XX0X	auto start off
		XX1X	auto start on
		XXX0	beep off
		XXX1	beep on
		XXXX0	internal air admittance valve off
		XXXX1	internal air admittance valve auto
		XXXX2	internal air admittance valve on
OUT_SP_1	set vacuum	XXXX	unit corresponding to default settings (mbar/hPa/Torr); see respective operation for parameter range
OUT_SP_V	set vacuum with venting	XXXX	unit corresponding to default settings (mbar/hPa/Torr); see respective operation for parameter range
OUT_SP_2	motor speed	XXX	motor speed in % (1-100%) or HI or 101 allowed
OUT_SP_3	start-up pressure	XXXX	unit corresponding to default settings (mbar/hPa/Torr); see respective operation for parameter range
OUT_SP_4	delay time	XX:XX	hh:mm (hours:minutes)
OUT_SP_5	switch-off pressure	XXXX	unit corresponding to default settings (mbar/hPa/Torr); see respective operation for parameter range
OUT_SP_6	switch-off time	XX:XX	hh:mm (hours:minutes)
OUT_SP_PL	open program	X	program 0.....9
OUT_SP_PS	store program	X	program 0.....9
OUT_SP_P1y	time	XX:XX:XX oder +XX:XX:XX	total runtime until program step y (0.....9) or time for program step y (0.....9) (additive)
OUT_SP_P2y	pressure	XXXX	pressure in program step y (0.....9) ; unit corresponding to default settings (mbar/hPa/Torr)
OUT_SP_P3y	air admittance valve	0	no air admittance valve in program step y (0...9)
		1	air admittance valve in program step y (0.....9)

Command	Operation	Parameter	Description
OUT_SP_P4y	step	0	no Step in program step y (0.....9)
		1	Step in program step y (0.....9)
OUT_SP_P5y	auto	0	no Auto in program step y (0.....9)
		1	Auto in program step y (0.....9)
		2	Auto in program step y (0.....9)
START	---	---	start process control
STOP	---	0	stop and delete error
		1	stop
		2	stop and store set vacuum
REMOTE**	remote operation	0	remote off
		1	remote on
** <i>For operation by remote (remote on/off), the user must ensure that no hazardous situation can arise in the system. Especially when due to activated remote direct process control is impossible.</i>			
ECHO***		0	echo off
		1	echo on, write commands with reply value
*** <i>With command ECHO 1 a return value can be activated at write commands. A return value is only given if the command is performed correctly.</i>			
CVC	---	2	CVC 2000 commands
		3	CVC 3000 commands****
**** <i>After being switched on, the controller is in CVC 2 mode by default. Send CVC 3 and STORE to permanently set the controller RS 232C commands to the extended set CVC 3000.</i>			
OUT_VENT	---	0	air admittance valve closed
		1	air admittance valve open
		2	venting until atmospheric pressure (1060 mbar at maximum)
STORE	store settings		store settings permanently, if „ECHO = 1“ after realization
OUT_SENSOR	---	1	internal sensor, if connected; alternatively external sensor.
		2...9	external sensors (if connected)

10.3 Ordering information

Ordering information CVC	Vacuum controller	Order-N°
	CVC 3000 table top version	20683160
	CVC 3000 built-in version	20636595
	CVC 3000 + VSP 3000 (package for fine vacuum control)	20635983
Ordering information spare parts	Spare parts	Order-N°
	Vacuum sensor (vacuum gauge head)	
	VSK 3000, 1080-0,1 mbar	20640530
	VSP 3000 (Pirani), $1 \times 10^3 - 1 \times 10^{-3}$ mbar	20636163
	VACUU·VIEW, Vacuum gauge with integrated vacuum sensor, 1100-0.1 mbar	20683220
	VACUU·VIEW extended, Vacuum gauge with integrated vacuum sensor, 1100-0.001 mbar	20683210
	VACUU·SELECT Sensor	20700020
	VACUU·SELECT Sensor without air valve	20700021
	In-line isolation valve (electromagnetic vacuum valve)	
	VV-B 6, 24 VDC, VACUU·BUS	20674290
	VV-B 6C, 24 VDC, VACUU·BUS	20674291
	VV-B 15C, KF 16, VACUU·BUS	20674210
	VV-B 15C, KF 25, VACUU·BUS	20674215
	Coolant valve VKW-B, VACUU·BUS	20674220
	Air admittance valve VBM-B / KF 16, VACUU·BUS	20674217
	Y adapter VACUU·BUS	20636656
	Extension cable VACUU·BUS, 2m	20612552
	Wall duct VACUU·BUS	20636153
	Cable RS 232C, 9-poles, Sub-D	20637837
	Installation kit CVC 3000 (spring clips + screws)	20636593
	Level sensor (for round bottom flask 500 ml)	20699908
	Digital I/O interface module VACUU·BUS	20636228
	Analog I/O interface module VACUU·BUS	20636229
	Analog I/O interface module 4–20mA/0–10V VACUU·BUS	20635425
	Vacuum management module VMS-B, 100-230 V, 3.5 A, CEE	20676030
Ordering information VACUU·CONTROL®	Remote control	Order-N°
	VACUU·CONTROL® WLAN version	20683110
	VACUU·CONTROL® LAN version	20683120

Ordering information
accessories

Accessories	Order-N°
Selection knob	20612091
Plug-in rubber foot	20638901
Spring clip	20636782
Wall power supply plug 30 W, 24 V; with adapters	20612090
Wall power supply plug 25 W, 24 V; with adapters	20612089
Hose nozzle	20636045
Hose	20636046
Locking ring 10 mm for knurled nut M14 x 1 (637657)	20637658
Round head screw 4 x 18	20636947
O-ring 28 mm x 2 mm	20636975
Knurled nut M14 x 1 for hose fitting DN ^x 10/8mm, with-out locking ring	20637657

^x conversion - example: $d_i = 10 \text{ mm} = \text{DN } 10$

Source of supplyInternational sales
offices and
specialized trade


Purchase original accessories and spare parts from your specialized distributor or through international sales offices of **VACUUBRAND GMBH + CO KG**.



- ⇒ Information about the complete product range are available in the current [product catalog](#).
- ⇒ For orders, questions about vacuum control and optimal accessories, please contact your specialized distributor or an [international sales office](#) of **VACUUBRAND GMBH + CO KG**.

10.4 Service

Service range Take advantage of the comprehensive service range of **VACUUBRAND GMBH + CO KG**.

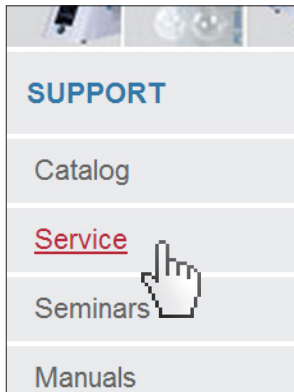

Service in detail

- Product guidance and practical solutions,
- fast delivery of spare parts and accessories,
- professional maintenance,
- immediate repairs processing,
- service on the spot (available upon request),
- [calibration](#) (DAkkS accredited),
- return, disposal.

⇒ Please visit our website for further information:
www.vacuubrand.com.

Service handling

Meet the terms of
service

1. Contact your local dealer or our service department¹.
2. Request a RMA number for your order.
3. Clean your product thoroughly and if necessary decontaminate it professionally.
4. Please fill in the form [Health and Safety Clearance](#) completely
5. Return your product including:
 - RMA number,
 - repair order,
 - form ***Health and Safety Clearance***,
 - short error description.

Send in your product
(return)



- ⇒ Reduce downtime, speed up the handling. Keep the required data and documents ready when contacting the service department.
- ▶ Your order can be quickly and easily processed.
 - ▶ Hazards can be excluded.
 - ▶ A short description or photos may help for error location.

¹ -> Phone: +49 9342 808-5660, Fax: +49 9342 808-5555,
 Mail to: service@vacuubrand.com

10.5 Glossary

HI mode	scores maximum pumping speed and low ultimate vacuum with the pump and optimum speed for the respective pressure (automatic speed reduction at ultimate vacuum).
Hysteresis	Regulates control performance of 2-point control in mode Vac control and Program. The hysteresis determines the threshold to which the actual value may differ from the setpoint. A too small hysteresis value leads to a frequent switching cycle. A too large hysteresis value leads to imprecise vacuum control.
Peltronic®	Electronic emission condenser; the Peltronic® condenses solvent vapors without external coolant such as water or dry ice. Cooling is achieved by Peltier elements. All wetted materials are highly resistant against chemicals.
Periphery equipment	in this manual: accessories and apparatus connected to the vacuum system such as vacuum valves, vacuum pumps and recipients; see also chapter 4.2.3 VACUU·BUS® .
Quick adaption	during running operation an operation mode can be tuned without calling up the corresponding operation menu. Usable for the modes Vac control – set vacuum adaption and Pump down – VARIO® motor speed adaption .
VACUU·BUS	digital communication system of VACUUBRAND . Possible components are: pressure/vacuum sensors, valves, level sensors, I/O modules; VARIO® pumps. When connecting several VACUU·BUS components of the same type it is necessary to regard that these components require different address numbers for communication; → see also Address assignment (configuration) on page 85 .
VACUU·CONTROL®	web-based remote control enables the monitoring and control of vacuum pumping units via computers or mobile devices such as Smartphones. With the new LAN or WLAN adapter all pumping units and vacuum systems equipped with the CVC 3000 vacuum controller or a DCP 3000 vacuum gauge can be integrated into a computer network.
VMS-B module	The Vacuum-Management-System module VMS-B switches a vacuum pump according to actual demand from one or two applications. It is operated by one or two vacuum controllers CVC 3000. If two CVC 3000 are connected to the VMS-B it switches off the pump only if both applications do not need a vacuum supply anymore

10.6 Index

A			
Abbreviations.....	11	E	
Action step.....	10	EC Declaration of Conformity.....	121
Active reset.....	96	Edit program.....	64
Adapt set vacuum.....	55	Electrical connection.....	29
Additional icons.....	10	Environmental protection.....	20
Additional notes.....	9	Error display.....	40,90
Address assignment.....	85	Examples of use.....	27
Address table VACUU•BUS.....	88	Explanation of usage conditions X ..	18
Adjustment at		Explosion danger.....	15
atmospheric pressure.....	100	explosive mixtures.....	15
Adjustment at reference pressure ..	102	F	
Adjustment under vacuum.....	101	Fault – Cause – Remedy.....	92
Analog I/O module.....	88	Fault indication.....	40
Assigned address numbers.....	85	fine vacuum control.....	104
ATEX approval.....	17	Firmware update.....	84
ATEX category.....	17	First steps.....	6
ATEX VARIO pump.....	88	First steps on delivery status.....	6
Audio signal (beep).....	40	Foreseeable misuse.....	13
Automatic reset.....	96	Functionality.....	23
Auto mode.....	48	Function menu.....	82
Auto start function.....	78	G	
B		Goods arrival.....	21
Back (return).....	43	H	
Bar graphic.....	37	Handling.....	42
bar marking.....	42	Handling CVC 3000.....	42
bench-top type.....	25	Health and Safety Clearance.....	18
built-in version.....	26	Hysteresis.....	60,61
C		I	
Call-up mode menu.....	47	Improper use.....	12,13
Change operation mode.....	51	Included materials.....	21
Cleaning and maintenance.....	99	Initialize frequency converter.....	83
Condensate.....	16	Input (data entry).....	43
configuration.....	85	Installation.....	25
Configuration menu.....	77	Installation conditions.....	25
Connection examples.....	32	int. Air V.....	83
Connect vacuum line.....	31	Intended use.....	12
Contact.....	8	Interface.....	11
Content selection.....	83	interface commands.....	107
Continuous venting.....	50	Internal air admittance valve.....	83
Control panel keys.....	35	K	
Copyright.....	7	Key combinations.....	36
Country-specific		L	
Interchangeable plug.....	29	Load Default.....	97
Creating a new program.....	67	Load factory settings.....	97
CVC 2000.....	108	M	
CVC 3000.....	11	Menu – Auto mode.....	60
D		Menu display in general.....	41
Defaults (standard).....	78	menu items (Configuration).....	78
Differential pressure.....	89	menu items (Function).....	83
Differential pressure measurement ..	89	Menu – Program.....	61
Digitale Druckanzeige.....	91	Menu – Pump down.....	58
digital pressure gauge.....	37	Menu – Vac control.....	59
Direct installation.....	26	Menu VACUULAN.....	62
Display graphic (curve).....	53	Mode.....	47
Display icons.....	38		

Mode menu.....	48	Select language.....	46
Momentarily venting	50	Select language and units	6
Motor speed.....	56	Select operation mode.....	47
N		Select pressure unit.....	46
Navigation.....	42	Sensor adjustment.....	79
O		Sensor readjustment	100
Open/Change program.....	63	Sensor selection	80
Operating elements	35	Service.....	117
Operation.....	42,45	shortcuts	36
Operation menus	57	Signal sounds	40
Operation modes	24	Specification and features	23
optimize vacuum control.....	28	Specified content.....	78,83
Optimizing operation mode.....	57	Start controlling.....	49
Ordering information.....	115	Start Regelung.....	49
P		Store program.....	70
Particles, liquids, dust.....	16	Sub-D	22
Peripherals	11	Sub-D Einbaustecker.....	107
Pin assignment (RS232).....	107	Submenu Configuration.....	41
Possible address configurations.....	88	Submenu Display	79
Power supply	29	Submenu RS232	81
Prepare sensors	89	Submenus	42
Pressure display.....	37	Submenu Sensors	80
Pressure history.....	53	Submenu Vacuubus	85
Product comparison.....	105	Switch-on CVC 3000	45
Product description.....	21	Switch-on/-off.....	45
Program.....	48	T	
Program display at operation.....	71	Table top version	25
program editor	64	Target groups.....	14
Program examples	74	Technical data.....	103
Program functions	63	Technical information.....	103
Program memory.....	72	Technical support.....	90
Protective clothing	15	temporary buffer	72
Pump down.....	48	Term definition	11
Q		U	
Quality standards.....	15	US/CAN Certificate.....	123
R		User permissions.....	14
Rating plate	106	V	
Read command	108	Vac control.....	48
Reference sensors	80	VACUU•BUS.....	33
Remote	81	VACUU•BUS accessories.....	34
Requirements for services.....	19	VACUU•BUS components.....	34
Reset	96	VACUU•BUS principle	33
Reset Remote.....	81,93	VACUU•CONTROL	16
Residual energy.....	16	VACUULAN	48,62
Responsibility Assignment Matrix.....	14	Vacuum connection	31
RMA-N°	19	Vacuum controller CVC 3000	21
RMA number.....	117	vacuum port.....	31
RS-232	81	VACUU•VIEW.....	34,88,89,115
RS232 port	40	VACUU•VIEW extended	34,88,115
S		Vario init.....	83
Safety and service	18	Venting (VENT).....	49
safety instructions.....	12	W	
Safety symbols	9	Warning levels	8
sales offices.....	116	Warning triangle	90
Sample form	76	Wetted parts	106
Scope of supply	21	Write command	113
Selection.....	42		
Selection knob.....	35		

10.7 Certifications

10.7.1 EC Declaration of Conformity

EG-Konformitätserklärung für Maschinen EC Declaration of Conformity of the Machinery Déclaration CE de conformité des machines



Hersteller / Manufacturer / Fabricant:

VACUUBRAND GMBH + CO KG · Alfred-Zippe-Str. 4 · 97877 Wertheim · Germany

Hiermit erklärt der Hersteller, dass das Gerät konform ist mit den Bestimmungen der Richtlinien:

Hereby the manufacturer declares that the device is in conformity with the directives:

Par la présente, le fabricant déclare, que le dispositif est conforme aux directives:

- 2014/35/EU
- 2014/30/EU
- 2014/34/EU (außer / except / sauf : 20635028)
- 2011/65/EU, 2015/863

Vakuum-Controller / Vacuum controller / Régulateur de vide:

Typ / Type / Type: **CVC 3000**

Artikelnummer / Order number / Numéro d'article: **20635027, 20635028, 20636310, 20683160, 22615721**

Seriennummer / Serial number / Numéro de série: Siehe Typenschild / See rating plate / Voir plaque signalétique

Angewandte harmonisierte Normen / Harmonized standards applied / Normes harmonisées utilisées:

EN ISO 12100:2010 (ISO 12100:2010), EN 61010-1:2010 + A1:2019 + A1:2019/AC:2019

(IEC 61010-1:2010 + COR:2011 + A1:2016, modifiziert / modified / modifié + A1:2016/COR1:2019)

EN IEC 61326-1:2021 (IEC 61326-1:2020)

EN 1127-1:2019; EN ISO 80079-36:2016 (ISO 80079-36:2016) (außer / except / sauf : 20635028)

EN IEC 63000:2018 (IEC 63000:2016)

Bevollmächtigter für die Zusammenstellung der technischen Unterlagen / Person authorised to compile the technical file / Personne autorisée à constituer le dossier technique:

Dr. Constantin Schöler · VACUUBRAND GMBH + CO KG · Germany

Ort, Datum / place, date / lieu, date: Wertheim, 30.08.2024

(Dr. Constantin Schöler)

Geschäftsführer / Managing Director / Gérant

ppa.

(Jens Kaibel)

Technischer Leiter / Technical Director /
Directeur technique

VACUUBRAND GMBH + CO KG

Alfred-Zippe-Str. 4
97877 Wertheim

Tel.: +49 9342 808-0

Fax: +49 9342 808-5555

E-Mail: info@vacuubrand.com

Web: www.vacuubrand.com

10.7.2 UKCA Declaration of Conformity

Declaration of Conformity



Manufacturer:

VACUUBRAND GMBH + CO KG · Alfred-Zippe-Str. 4 · 97877 Wertheim · Germany

Hereby the manufacturer declares that the device is in conformity with the directives:

- Electrical Equipment (Safety) Regulations 2016 (S.I. 2016 No. 1101, as amended by S.I. 2019 No. 696)
- Electromagnetic Compatibility Regulations 2016 (S.I. 2016 No. 1091, as amended by S.I. 2019 No. 696)
- The Equipment and Protective Systems Intended for Use in Potentially Explosive Atmospheres Regulations 2016 (S.I. 2016 No. 1107, as amended by S.I. 2019 No. 696) (except: 20635028)
- The Restriction of the Use of Certain Hazardous Substances in Electrical and Electronic Equipment Regulations 2012 (S.I. 2012 No. 3032)

Vacuum controller:

Type: **CVC 3000**

Order number: **20635027, 20635028, 20636310, 20683160, 22615721**

Serial number: See rating plate

Designated standards applied:

EN ISO 12100:2010, EN 61010-1:2010+A1:2019, EN 61010-1:2010/A1:2019/AC:2019-04

EN 61326-1:2013

EN 1127-1:2019, EN ISO 80079-36:2016 (except: 20635028)

EN IEC 63000:2018

Person authorised to compile the technical file:

Dr. Constantin Schöler · VACUUBRAND GMBH + CO KG · Germany

Place, date: Wertheim, 30.08.2024

(Dr. Constantin Schöler)

Managing Director

ppa.

(Jens Kaibel)

Technical Director

VACUUBRAND GMBH + CO KG

Alfred-Zippe-Str. 4
97877 Wertheim



Tel.: +49 9342 808-0

Fax: +49 9342 808-5555

E-Mail: info@vacuubrand.com

Web: www.vacuubrand.com

10.7.3 US/CAN Certificate

Certificate		
Certificate no.	CU 72228817 01	
License Holder: VACUUBRAND GMBH + CO KG Alfred-Zippe-Str. 4 97877 Wertheim Deutschland	Manufacturing Plant: VACUUBRAND GMBH + CO KG Alfred-Zippe-Str. 4 97877 Wertheim Deutschland	
Test report no.: USA- 31880183 003	Client Reference: Dr. A. Wollschläger	
Tested to: UL 61010-1:2012 R7.19 CAN/CSA-C22.2 NO. 61010-1-12 + GI1 + GI2 (R2017) + A1		
Certified Product: Measurement and control device for vacuum	License Fee - Units	
Model : (1) VACUU VIEW; (2) VACUU VIEW extended;	7	
Designation : (3) VACUU SELECT; (4) VACUU SELECT complete;		
(5) VACUU SELECT Sensor;		
(6) VSP 3000; (7) CVC 3000; (8) VSK 3000;		
(9) VSK PV; (10) DCP 3000		
Rated Voltage: DC 24V; class III (all devices)		
Rated Power : (1+2) 1.3W; (3) 5.0W; (4) 13W; (5) 1.2W;		
(6) 1.6W; (7+10) 3.4W; (8+9) 0.12W		
Degree of : (7+10) IP20/Type 1 (UL50E)		
Protection : (3+4) IP40/Type 1 (UL50E)		
(5) IP41/Type 2 (UL50E)		
(1+2+6+8+9) IP54/Type 5 (UL50E)		
Appendix: 1, 1-13		7
Licensed Test mark:  C US	Date of Issue (day/mo/yr) 09/02/2023	
TUV Rheinland of North America, Inc., 12 Commerce Road, Newtown, CT 06470, Tel (203) 426-0888 Fax (203) 426-4009		

10.7.4 Declaration of Conformity – China RoHS 2

VACUUBRAND®

DECLARATION OF CONFORMITY – China RoHS 2

VACUUBRAND GMBH + CO KG has made reasonable efforts to ensure that hazardous materials and substances may not be used in its products.

In order to determine the concentration of hazardous substances in all homogeneous materials of the subassemblies, a “Product Conformity Assessment” (PCA) procedure was performed. As defined in GB/T 26572 the “Maximum Concentration Value” limits (MCV) apply to these restricted substances:

- Lead (Pb): 0.1%
- Mercury (Hg): 0.1%
- Cadmium (Cd): 0.01%
- Hexavalent chromium (Cr(+VI)): 0.1%
- Polybrominated biphenyls (PBB): 0.1%
- Polybrominated diphenyl ether (PBDE): 0.1%

Environmentally Friendly Use Period (EFUP)

EFUP defines the period in years during which the hazardous substances contained in electrical and electronic products will not leak or mutate under normal operating conditions. During normal use by the user such electrical and electronic products will not result in serious environmental pollution, cause serious bodily injury or damage to the user's assets. The Environmentally Friendly Use Period for VACUUBRAND products is 40 years.



MATERIAL CONTENT DECLARATION FOR VACUUBRAND PRODUCTS						
有毒有害物质或元素 Hazardous substances						
部件名称 Part name	铅 Pb	汞 Hg	镉 Cd	六价铬 Cr(+VI)	多溴联苯 PBB	多溴二苯醚 PBDE
包装 Packaging	O	O	O	O	O	O
塑料外壳 / 组件 Plastic housing / parts	O	O	O	O	O	O
真空油 Vacuum oil	O	O	O	O	O	O
电池 Battery	O	O	O	O	O	O
玻璃 Glass	X	O	O	O	O	O
电子电气组件 Electrical and electronic parts	X	O	O	O	O	O
控制器 / 测量设备 Controller / measuring device	X	O	O	O	O	O
金属外壳 / 组件 Metal housing / parts	X	O	O	O	O	O
电机 Motor	X	O	O	O	O	O
配件 Accessories	X	O	O	O	O	O
此表格是按照SJ/T 11364-2014中规定所制定的。 This table is created according to SJ/T 11364-2014.						

Declaration of Conformity – China RoHS 2

V5_September 2022

Copyright 2022

VACUUBRAND®

- O: 表示该有毒有害物质在该部件所有均质材料中的含量均在GB/T 26572规定的限量要求以下。
O: Indicates that the above mentioned hazardous substance contained in all homogeneous materials of the part is below the required limit as defined in GB/T 26572.
- X: 表示该有毒有害物质至少在该部件某一均质材料中的含量超出GB/T 26572规定的限量要求。
X: Indicates that the above mentioned hazardous substance contained in at least one of the homogeneous materials of this part is above the required limit as defined in GB/T 26572.

电池、玻璃器皿和配件可能不属于所附设备所包含的内容，它们可能有各自单独的EFUP标记和/或可能正在维护其部件EFUP标记的更新。

Batteries, glassware and accessories might not be content of the enclosed device and may have its own EFUP-marking and/or might be maintaining parts with changing EFUP-marking.

除上表所示信息外，还需声明的是，这些部件并非是有意图用铅（Pb）、汞（Hg）、铬（Cd）、六价铬（Cr(+VI)）、多溴联苯（PBB）或多溴二苯醚（PBDE）来制造的。

Apart from the disclosures in the above table, the subassemblies are not intentionally manufactured or formulated with lead (Pb), mercury (Hg), cadmium (Cd), hexavalent chromium (Cr+VI), polybrominated biphenyls (PBB), and polybrominated diphenyl ethers (PBDE).

Products manufactured by VACUUBRAND may enter into further devices (e.g., rotary evaporator) or can be used together with other appliances (e.g., usage as booster pumps).


With these products and appliances in particular, please note the EFUP labeled on these products.

VACUUBRAND will not take responsibility for the EFUP of those products and appliances.

Place, date: Wertheim, 06 September 2022



(Dr. Constantin Schöler)
Managing Director




ppa. (Jens Kaibel)
Technical Director

VACUUBRAND GMBH + CO KG

Alfred-Zippe-Str. 4
97877 Wertheim
Germany

Tel.: +49 9342 808-0
Fax: +49 9342 808-5555
E-Mail: info@vacuubrand.com
Web: www.vacuubrand.com

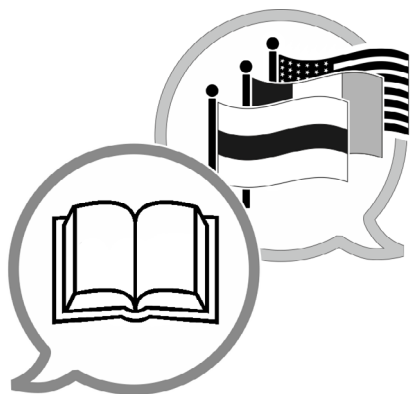

www.vacuubrand.com/manuals

Manufacturer:

VACUUBRAND GMBH + CO KG
Alfred-Zippe-Str. 4
97877 Wertheim
GERMANY

Phone:

Head office +49 9342 808-0

Sales +49 9342 808-5550

Service +49 9342 808-5660

Fax: +49 9342 808-5555

Email: info@vacuubrand.com

Web: www.vacuubrand.com